

SIEMENS

DICOM Conformance Statement

syngo® MR E11E

Last Change: 2020-11-20

1 Conformance Statement Overview

“syngo® is an application framework for end hospital medical applications for imaging modalities. syngo supports Storage and Transfer of images utilizing the DICOM “Storage Service Class”, the display of data and retrieval of images from DICOM Archives utilizing the DICOM “Query/Retrieve Service Class”. Workflow Management is supported by querying worklists from RIS and returning information about the procedure performed. Furthermore the Import from and export to DICOM CD/DVD media is supported. Printing of viewing results is provided with Print Management Services.

Table 1 - Network Services

SOP Classes	User of Service (SCU)	Provider of Service (SCP)
Verification		
Verification	Yes	Yes
Transfer (Image SOP Class)		
CR Image Storage	Yes	Yes
CT Image Storage	Yes	Yes
Enhance CT Image Storage	Yes	Yes
DX Image Storage for Processing	Yes	Yes
DX Image Storage for Presentation	Yes	Yes
Digital MG Image Storage for Processing	Yes	Yes
Digital MG Image Storage for Presentation	Yes	Yes
Digital Intra-oral X-Ray Image Storage for Presentation	Yes	Yes
Digital Intra-oral X-Ray Image Storage for Processing	Yes	Yes
MR Image Storage	Yes	Yes
Enhanced MR Image Storage	Yes	Yes
Enhanced MR Colored Image Storage	Yes	Yes
X-Ray 3D Angiographic Image Storage	Yes	Yes
Breast Tomosynthesis Image Storage	Yes	Yes
NM Image Storage	Yes	Yes
PET Image Storage	Yes	Yes
RT Dose Storage	Yes	Yes
RT Image Storage	Yes	Yes
SC Image Storage	Yes	Yes
Multiframe Single Bit SC Image Storage	Yes	Yes
Multiframe Grayscale Byte SC Image Storage	Yes	Yes
Multiframe Grayscale Word SC Image Storage	Yes	Yes
Multiframe True Color SC Image Storage	Yes	Yes
US Image (retired)	Yes	Yes
US Multiframe Image (retired)	Yes	Yes
US Multiframe Image Storage	Yes	Yes
US Image Storage	Yes	Yes
X-Ray RadioFluoroscopic Image Storage	Yes	Yes
X-Ray Angiographic Image Storage	Yes	Yes
Segmentation Storage	Yes	Yes
Transfer (Non-image SOP Class)		
MR Spectroscopy Storage	Yes	Yes
Grayscale Softcopy Presentation State Storage	Yes	Yes
RT Structure Set Storage	Yes	Yes
RT Plan Storage	Yes	Yes

RT Ion Plan Storage	Yes	Yes
RT Ion Beams Treatment Record Storage	Yes	Yes
RT Brachy Treatment Record Storage	Yes	Yes
RT Treatment Summary Record Storage	Yes	Yes
12-lead ECG Waveform Storage	Yes	Yes
Ambulatory ECG Waveform Storage	Yes	Yes
Basic Voice Audio Waveform Storage	Yes	Yes
Cardiac Electrophysiology Waveform Storage	Yes	Yes
General ECG Waveform Storage	Yes	Yes
Hemodynamic Waveform Storage	Yes	Yes
RAW Data Storage	Yes	Yes
Spatial Registration Storage	Yes	Yes
Spatial Fiducials Storage	Yes	Yes
Surface Segmentation Storage	Yes	Yes
Basic Text SR	Yes	Yes
Enhanced SR	Yes	Yes
Comprehensive SR	Yes	Yes
Procedure Log	Yes	Yes
Mammography CAD SR	Yes	Yes
Key Object Selection Document	Yes	Yes
Chest CAD SR	Yes	Yes
X-Ray Radiation Dose SR	Yes	Yes
Encapsulated PDF	Yes	Yes
Transfer (Private SOP Class)		
Syngo Non-Image Storage	Yes	Yes
Workflow Management		
Modality Performed Procedure Step SOP Class	Yes	No
Modality Worklist Information Model - FIND	Yes	No
Storage Commitment Push Model SOP Class	Yes	Yes
Query/Retrieve		
Patient Root Q/R Information Model - FIND	Yes	Yes
Patient Root Q/R - Information Model - MOVE	Yes	Yes
Patient Root Q/R - Information Model - GET	Yes (See Note 1)	Yes
Study Root Q/R - Information Model - FIND	Yes	Yes
Study Root Q/R - Information Model - MOVE	Yes	Yes
Study Root Q/R - Information Model - GET	Yes (See Note 1)	Yes
Patient/Study Only Q/R - Information Model FIND	Yes	Yes
Patient/Study Only Q/R - Information Model MOVE	Yes	Yes
Patient/Study Only Q/R - Information Model GET	Yes (See Note 1)	Yes
Print Management		
Basic Grayscale Print Management Meta	Yes	No
Print Job	Yes	No
Presentation LUT	Yes (for Grayscale)	No

Note 1: The DICOM C GET Service is supported in addition by syngo Study Transfer application.

Table 2 - Media Services

Media Storage Application Profile	Write Files (FSC or FSU)	Read Files (FSR)
Compact Disk - Recordable		
General Purpose on CD-R and DVD	Yes (see Note 1)	Yes
Basic Cardiac X-Ray on CD-R	Yes (see Note 2)	Yes
1024 X-Ray on CD-R	Yes	Yes
DVD		
1024 X-Ray on DVD	Yes	Yes
General Purpose DVD with JPEG	Yes	Yes

Note 1: with uncompressed setting

Note 2: with "resize" (512x512) active and only cine multi-frames included

Table 3 - Implementation Identifying Information

Name	Value
Application Context Name	1.2.840.100008.3.1.1.1
Implementation Class UID	1.3.12.2.1107.5.9.20000101
Implementation Version Name	"VE11E"

2 Table of Contents

1	Conformance Statement Overview	2
2	Table of Contents	5
3	Introduction.....	8
3.1	Scope and Field.....	8
3.2	Audience	8
3.3	Remarks	9
3.4	Definitions, Terms and Abbreviations.....	9
3.5	References	10
4	Networking.....	11
4.1	Implementation Model	11
4.1.1	Application Data Flow	11
4.1.2	Functional Definitions of Application Entities.....	14
4.1.3	Sequencing of Activities.....	15
4.2	Application Entity Specification.....	17
4.2.1	Verification SCU AE Specification	17
4.2.2	Storage SCU AE Specification	19
4.2.3	Storage SCP AE Specification.....	24
4.2.4	Query/Retrieve SCU Specification.....	33
4.2.5	Query/Retrieve SCP Specification.....	39
4.2.6	Print SCU Specification	46
4.2.7	Worklist SCU AE.....	55
4.2.8	Modality PPS SCU AE.....	62
4.3	Network Interfaces	69
4.3.1	Physical Network Interface	69
4.3.2	Additional Protocols.....	69
4.3.3	IPv4 and IPv6 Support.....	69
4.4	Configuration.....	69
4.4.1	AE Title/Presentation Address Mapping.....	69
4.4.2	Parameters	71
5	(DICOM) Media Interchange / Offline Media Interchange	73
5.1	Implementation Model	73
5.1.1	Application Data Flow Diagram	73
5.1.2	Functional Definitions of AEs.....	73
5.1.3	Activities.....	74
5.1.4	Implementation Identifying Information.....	74
5.2	AE Specifications	75
5.2.1	DICOM Archive Specification	75
5.3	Augmented and Private Application Profiles.....	78
5.4	Media Configuration.....	79
5.4.1	Single- / Multi-Session CD burning.....	79
5.4.2	Auto-Labeling.....	79

6	Support of Extended Character Sets	80
7	Security	83
7.1.1	Security Transport Connection Profiles	83
8	Annexes	86
8.1	MR Image IOD	86
8.1.1	Patient Module	86
8.1.2	General Study Module	86
8.1.3	Patient Study Module	86
8.1.4	General Series Module	87
8.1.5	Frame of Reference Module	88
8.1.6	General Equipment Module	88
8.1.7	General Image Module	88
8.1.8	Image Plane Module	89
8.1.9	Image Pixel Module	89
8.1.10	Contrast/Bolus Module	89
8.1.11	MR Image Module	90
8.1.12	MR Private Diffusion Module	91
8.1.13	VOI LUT Module	91
8.1.14	SOP Common Module	91
8.2	MR Spectroscopy IOD	91
8.2.1	Patient Module	91
8.2.2	General Study Module	92
8.2.3	General Series Module	92
8.2.4	MR Series Module	92
8.2.5	Frame of Reference Module	92
8.2.6	General Equipment Module	92
8.2.7	Enhanced General Equipment Module	93
8.2.8	Shared Functional Groups	93
8.2.9	Per-frame Functional Groups	94
8.2.10	Multi-Frame Functional Groups Module	95
8.2.11	Multi-frame Dimension Module	95
8.2.12	Acquisition Context Module	95
8.2.13	MR Spectroscopy Module	95
8.2.14	Cardiac Synchronization Module	96
8.2.15	MR Spectroscopy Pulse Sequence Module	96
8.2.16	MR Spectroscopy Data Module	96
8.2.17	SOP Common Module	97
8.3	MR Evidence Document Templates	97
8.4	SIEMENS Private Non-Image IOD	97
8.4.1	Siemens Non-Image IOD – E-R Model	97
8.4.2	Siemens Non-Image IOD - Module Table	99
8.4.3	CSA Series Header Module	99
8.4.4	Siemens Non-Image IOD - Modules	99
8.5	Siemens Standard Extended Modules	101
8.5.1	CSA Image Header Module	101
8.5.2	MEDCOM Header Module	101
8.5.3	MEDCOM OOG Module	103
8.5.4	syngo Report Data	103
8.5.5	syngo Report Info	104
8.6	Registry of DICOM Data Elements	104
8.7	Standard Extension of all SOP Classes	105
8.7.1	Image Type	106

8.8	DICOM Print SCU – detailed status displays	110
8.8.1	Common Status Information	111
8.8.2	Additional Status Information – AGFA printers.....	114
8.8.3	Additional Status Information – Kodak PACS Link (formerly Imation).....	114
8.8.4	Additional Status Information – Kodak 1901	115
8.8.5	Additional Status Information – Kodak 2180/1120	115
8.8.6	Additional Status Information – Codonics.....	115
8.8.7	Additional DICOM Execution Status Information Evaluation.....	116
8.8.8	Additional DICOM Execution Status Information.....	116
Annex A: Index of Tables.....		118

3 Introduction

3.1 Scope and Field

This DICOM Conformance Statement refers to SIEMENS MR products using software *syngo*® MR E11E. The following table relates *syngo* MR E11E software versions to SIEMENS *syngo*® MR products.

Software Name	SIEMENS MR Product
syngo MR E11E	MAGNETOM Aera
syngo MR E11E	MAGNETOM Skyra
syngo MR E11E	MAGNETOM Prisma
syngo MR E11E	MAGNETOM Prisma-fit
syngo MR E11E	MAGNETOM Avanto-fit
syngo MR E11E	MAGNETOM Skyra-fit



The *syngo*® MR product is a “*syngo*®-speaking^a” Imaging Modality or workstation. The *syngo*® MR product is designed to be integrated into an environment of medical DICOM-based devices. The *syngo*® MR product DICOM network implementation acts as SCU and SCP for the DICOM Storage, Storage Commitment and Query/Retrieve services and as SCU for the DICOM Print, DICOM Basic Worklist and Modality Performed Procedure Step Services. Verification is supported in SCU (only via Service environment) and SCP role. Furthermore, the handling of offline media is supported as a FSC, FSU and FSR.

3.2 Audience

This document is intended for hospital staff, health system integrators, software designers or implementers. It is assumed that the reader has a working understanding of DICOM.

^a *syngo* is a registered trademark of Siemens AG

3.3 Remarks

The scope of this DICOM Conformance Statement is to facilitate integration between syngo and other DICOM products. The Conformance Statement should be read and understood in conjunction with the DICOM Standard [1]. DICOM by itself does not guarantee interoperability.

The Conformance Statement does, however, facilitate a first-level comparison for interoperability between different applications supporting compatible DICOM functionality.

This Conformance Statement is not supposed to replace validation with other DICOM equipment to ensure proper exchange of intended information. In fact, the user should be aware of the following important issues:

- The comparison of conformance statements is the first step towards assessing interconnectivity and interoperability between syngo and other DICOM conformant equipment.
- Test procedures should be defined and executed to validate the required level of interoperability with specific compatible DICOM equipment, as established by the healthcare facility.

syngo has participated in an industry-wide testing program sponsored by Integrating the Healthcare Enterprise (IHE) [2]. The IHE Integration Statement for syngo, together with the IHE Technical Framework, may facilitate the process of validation testing.

Siemens reserves the right to modify the design and specifications contained herein without prior notice. Please contact your local Siemens representative for the most recent product information.

3.4 Definitions, Terms and Abbreviations

Definitions, terms and abbreviations used in this document are defined within the different parts of the DICOM standard.

Additional Abbreviations and terms are as follows:

AE	DICOM Application Entity
AET	Application Entity Title
ASCII	American Standard Code for Information Interchange
CSE	Customer Service Engineer
DB	Database
DCS	DICOM Conformance Statement
DICOM	Digital Imaging and Communications in Medicine
FSC	File Set Creator
FSR	File Set Reader
FSU	File Set Updater
GSDF	Grayscale Standard Display Function
IHE	Integrating the Healthcare Enterprise
IOD	DICOM Information Object Definition
ISO	International Standard Organization
MPPS	Modality Performed Procedure Step
n. a.	not applicable
NEMA	National Electrical Manufacturers Association
O	Optional Key Attribute
PDU	DICOM Protocol Data Unit
R	Required Key Attribute
SCU	DICOM Service Class User (DICOM client)
SCP	DICOM Service Class Provider (DICOM Server)
SOP	DICOM Service-Object Pair
SPS	Scheduled Procedure Step
SR	Structured Report
TFT	Thin Film Transistor (Display)

TID	Template ID
U	Unique Key Attribute
UID	Unique Identifier
UTF-8	Unicode Transformation Format-8
VR	Value Representation

3.5 References

[1] Digital Imaging and Communications in Medicine (DICOM) Standard, available free at <http://medical.nema.org/>, NEMA PS 3^b

[2] Integrating the Healthcare Enterprise – IHE Radiology Technical Framework – www.ihe.net

• ^b The DICOM Standard is under continuous maintenance, the current official version is available at <http://dicom.nema.org>

4 Networking

4.1 Implementation Model

- **Verification**
The syngo DICOM Service Tool application requests Verification to proof the ability of a remote DICOM application to respond to DICOM messages. Responding to Verification requests from remote nodes is handled by the Storage SCP.
- **Storage**
The syngo DICOM implementation is able to initiate associations for Storage of DICOM Composite Information Objects to Remote AEs and to receive and respond to associations for Storage from Remote AEs.
- **StorageCommitment**
The syngo DICOM implementation is able to initiate requests for Storage Commitment Push (for previously sent DICOM Composite Information Objects) to Remote AEs and is able to receive and respond to Storage Commitment requests from Remote AEs.
- **Query/Retrieve**
The syngo DICOM application supports the Query/Retrieve services in a SCP role. Via the user interface, syngo supports Query/Retrieve as SCU to retrieve IODs to the local database.
- **Print**
The syngo DICOM implementation is able to initiate associations as Print Management SCU for printing of composed film-sheets with one or more DICOM Print AE.
- **Workflow**
The syngo will issue automated “broad” worklist queries and interactive “narrow” worklist queries as DICOM Modality Worklist SCU. The status of the procedure started and performed is communicated via MPPS, which is also supported in SCU role only. Radiation Dose information is also sent via MPPS.

4.1.1 Application Data Flow

The division of syngo into the separate DICOM Application Entities represents a somewhat arbitrary partitioning of functionality. For the purpose of this document they are organized in this manner to detail their independent logical functionality.

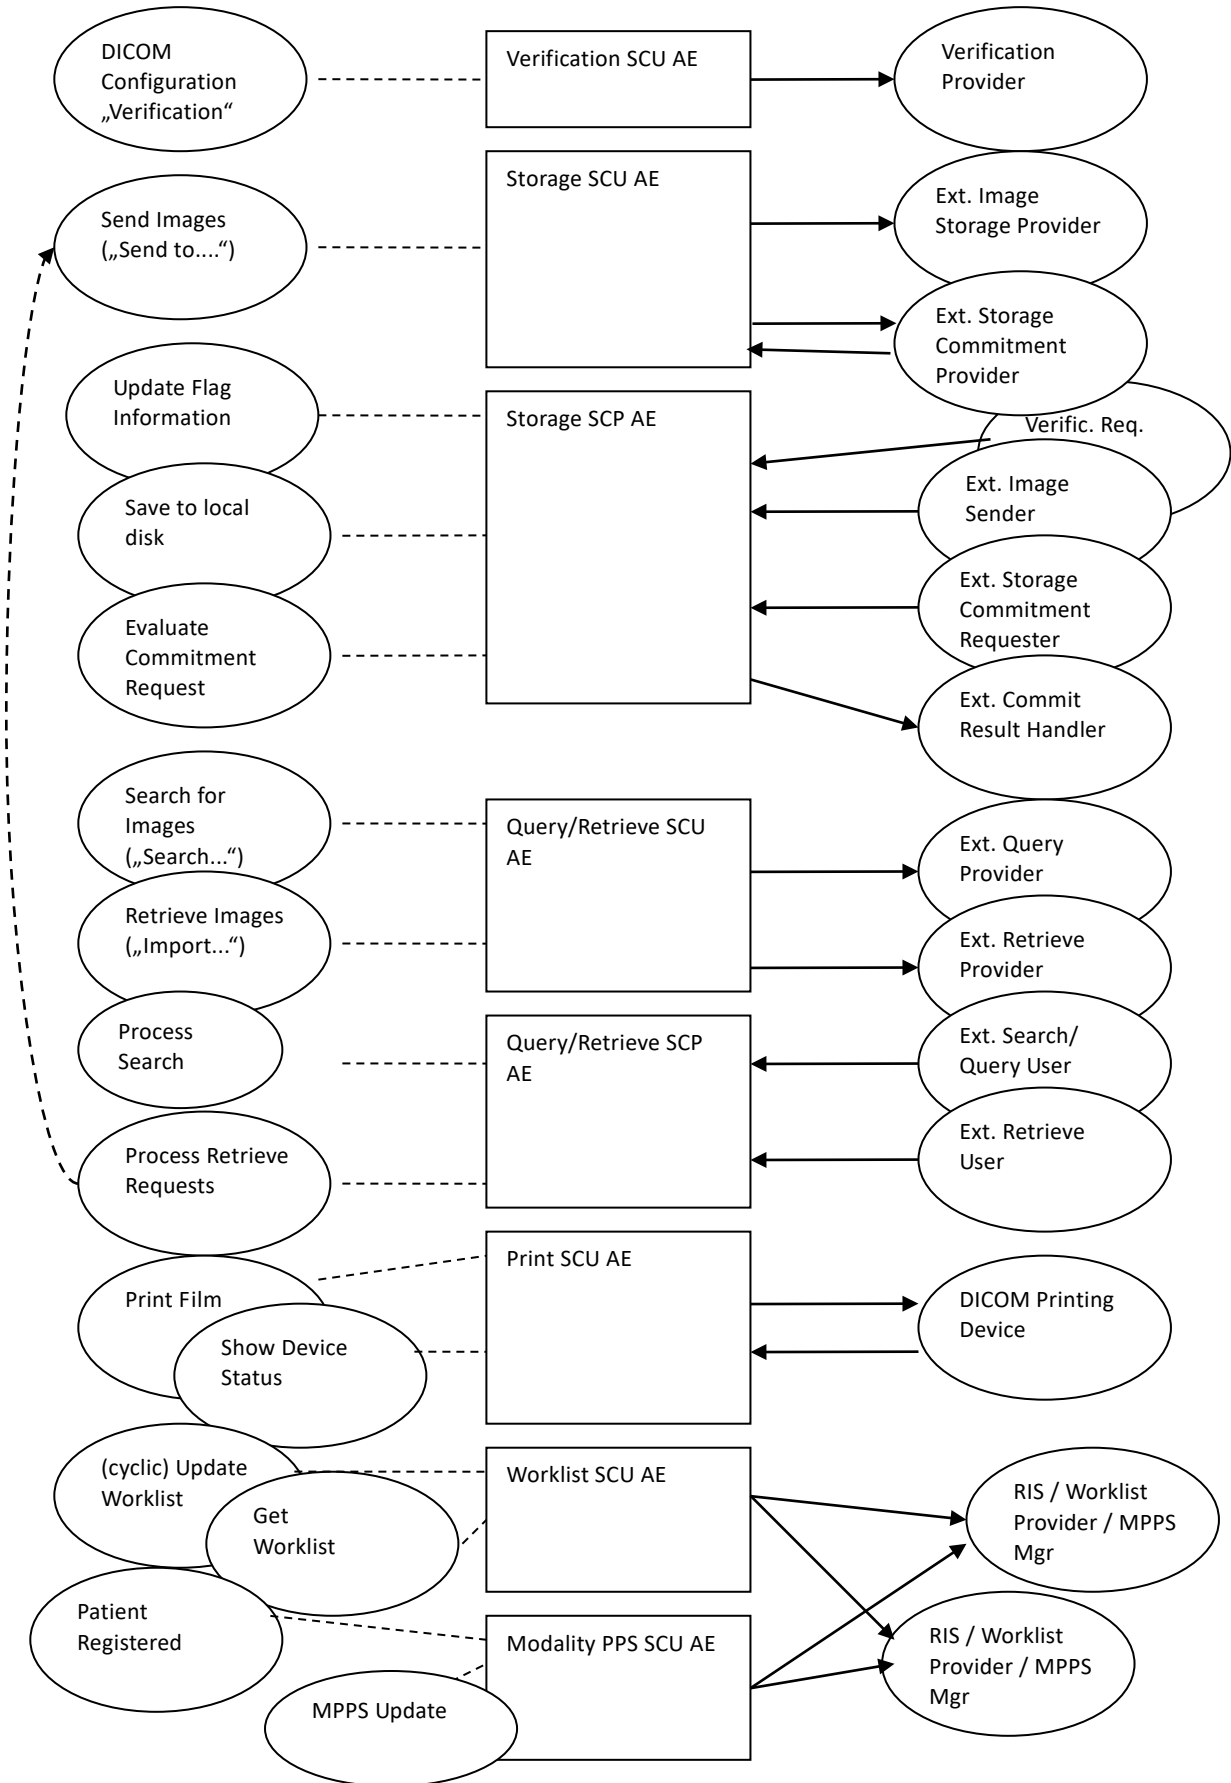


Figure 1: syngo DICOM Data Flow Diagram

- The syngo DICOM Service Tool application opens an association when a "verification" of a remote application is requested during a configuration session. This can be done when entering new data to configure a remote application or to verify existing configuration data.
- The Storage SCU AE can send Composite SOP Instances and automatically request Storage Commitment for sent SOP Instances, if configured.
The Storage SCU AE also handles incoming commitment status N-EVENT messages.
- The Storage SCP AE can receive incoming DICOM images and add them to the local database. It can respond to external Storage and Verification Requests as a Service Class Provider (SCP) for C-STORE and C-ECHO requests. The Storage SCP AE autonomously handles incoming Storage Commitment requests in SCP role and checks commitment status based on the local database and sends back the related commitment status in N-EVENT-REPORT messages.
The Storage SCP AE supports Composite SOP instances as indicated in chapter 1 "[Conformance Statement Overview](#)".
- The Query part of the Query/Retrieve SCU AE uses C-FIND to search a DICOM Database for Patient Study and Series information.
The Retrieve part of the Query/Retrieve SCU AE uses C-MOVE to initiate a DICOM transfer of composite objects to the local database.
- The Query SCP AE runs autonomously in the background and responds to incoming C-FIND requests based on the matches in the local database and supports retrieve of supported SOP Instances from the local database to a known retrieve destination.
- The Print SCU sends previously compiled, complete (virtual) film-sheets in 1:1 image mode (page mode) to the printer. The printer status is cyclically monitored by sending Status requests and/or awaiting asynchronous events.
- The Worklist SCU AE runs autonomously for cyclic "broad" query and issues C-FIND Worklist model requests. It can be manually triggered for most recent data. A "broad" query with user input can be triggered separately.
- The MPPS AE uses N-CREATE when registering an Acquisition patient and updates via N-SET with each run. The user can close MPPS interactively (triggers "final N-SET").

4.1.2 Functional Definitions of Application Entities

4.1.2.1 Functional Definition of Verification-SCU AE

The syngo DICOM Service Tool application opens an association when a "verification" of a remote application is requested during a configuration session. This can be done when entering new data for remote application configuration or to verify existing configuration data.

4.1.2.2 Functional Definition of Storage-SCU AE

The syngo Storage SCU is invoked by the job control interface that is responsible for processing network archival tasks. The job consists of data describing the composite image objects selected for storage and the destination. An association is negotiated with the destination application entity and the image data is transferred using the C-STORE DIMSE-Service. Status of the transfer is reported to the job control interface.

With each successfully completed send job, the syngo DICOM Application will populate the Storage Commitment Push Model Action Information from the SOP Instances sent. Then a Storage Commit Request is triggered, if configured. Depending on configuration, the syngo DICOM application will keep the association open for responses with a configurable time-out, or closes the association and expects responses on a different association that has to be established by the remote Storage Commitment SCP.

The commitment status derived from the related trigger response will be indicated in the related Status Flags of the related entity. It is possible to create triggers ("auto rules") from this event.

The Transaction UUIDs of the pending commitment request are kept "open" (Job-status is "waiting") for a configurable time (default: 1h). If the "open time" for a pending commitment request has elapsed w/o a related response from the provider, the Transaction UUID is removed and the related entities are indicated as "commit failed".

Open Transaction UUIDs of pending commitment requests are discarded after a reboot of the system. The related entities are indicated as "commit failed".

4.1.2.3 Functional Definition of Storage-SCP AE

The Storage SCP component of the syngo DICOM application is operating as background server process. The process starts when the machine is powered on and waits for Storage association requests. Upon accepting an association with a negotiated Presentation Context it starts to receive the Composite Image Objects and imports them to local database.

The Verification SCP is included in the Storage SCP.

The Storage Commitment SCP is running in background and is ready to receive requests when the system is started. Storage Commitment will be checked and returned against the SOP Classes received and kept in the local Storage of the syngo. The response will either be sent "on same" (association not closed by requester) or "on separate" association (requester closed association consecutive to positive request status).

4.1.2.4 Functional Definition of Query/Retrieve-SCU AE

The syngo DICOM Query/Retrieve SCU requests the remote Query/Retrieve SCP to perform a search and match to the keys specified in the request in order to display the results in the system's user interface. Depending on user action (Import) the syngo Query/Retrieve DICOM SCU sends a C-MOVE DIMSE service to initiate a C-STORE sub-operation on the SCP to start an image transfer from remote Storage SCU (running on Query/Retrieve SCP) to the system's Storage SCP.

4.1.2.5 Functional Definition of Query/Retrieve-SCP AE

The syngo DICOM Query/Retrieve SCP responds to C-FIND DIMSE services from remote SCU applications. Depending on further remote request, a C-GET or a C-MOVE involves the system's DICOM Query/Retrieve SCP application to initiate a C-STORE association to send image objects to a remote Storage SCP.

All components of the DICOM Query/Retrieve SCP application are operating as background server processes. The processes start when the machine is powered on and then respond to queries based on the records stored in its database.

4.1.2.6 Functional Definition of Print SCU AE

The Print SCU is invoked by the user interface to setup film-sheet layout and whenever an image is ready to be printed on film. The Print SCU will hold and maintain all data needed to compile a complete film-sheet from the data (images, layout, configuration) received. Whenever a film-sheet is ready to print the related data is used to supply the Information to the SOP Classes of the Print Management Service Class. A queue is maintained, in order to intermediately store several film-sheets in case of resource problems on printer. The SCU will only supply and require the mandatory SOP Classes of the Print Management Service Class.

4.1.2.7 Functional Definition of Worklist SCU AE

The worklist SCU ("broad query") is invoked from the patient browser user interface or by timer to request the worklist from a remote Information System (Modality Worklist Class SCP). The worklist SCP responses to the C-FIND query and scheduled imaging service requests (scheduled procedure steps) and patient demographic information will be "pulled" from the information system to the syngo modality. All information retrieved will be held in the scheduling database for usage during Patient Registration procedure.

Furthermore, the patient based Query dialog from the patient browser allows to enter specific matching criteria ("narrow query") for the worklist query. With the response data the Patient Registration dialog can be populated according availability within the worklist response identifier.

4.1.2.8 Functional Definition of Modality PPS SCU AE

With registering a Patient (i.e. a Scheduled Procedure Step from Worklist), the syngo DICOM application will create an MPPS Instance and communicate it to the MPPS Manager (SCP). It is configurable to set the states of all related MPPS to "Completed" when a patient is closed. Furthermore, a manual update can be performed with the MPPS user interface. From the user interface it is possible to set the state of the MPPS to "Completed" or "Discontinued". After that the DICOM application will no longer allow updates on the related MPPS Instance.

The syngo will not only allow a "1:1 -relationship" of Scheduled Procedure Steps and Performed Procedure Steps, but also supports the "simple group-case" (grouping several SPS of the same Requested Procedure) , "complex group-case" (grouping several SPS from different Requested Procedures) and "append case" from the respective IHE-scenarios.

The syngo will support creation of "unscheduled cases" by allowing MPPS Instances to be communicated for locally registered Patients.

4.1.3 Sequencing of Activities

4.1.3.1 Verification

Newly entered data have to be saved first, before a "verification" of these data is possible.

4.1.3.2 Storage

Prior to sending of SOP Instances the syngo Storage application is capable of invoking processing and resizing features in order to prepare image pixel contents into convenient formats for certain multi-vendor environments.

The Storage Commitment trigger is automatically derived from the successful completion of a Send Job.

4.1.3.3 Query/Retrieve

Retrieve of images is only possible if a result from a previous "Search..." operation exists and those entities can be selected for "Import".

The Query application will not "per se" request information on IMAGE level. The user can select a series and request image level information with the "Image List" function.

4.1.3.4 Workflow

The "narrow" (interactive) Worklist Query requires that sufficient matching keys or a unique matching key are/is entered before the query is issued. Only then a single response can be expected to complete the registration dialog.

An MPPS N-CREATE message is sent when a patient is registered. For procedure steps registered as "emergency" cases the MPPS N-CREATE is withheld until it is set to complete.

4.2 Application Entity Specification

4.2.1 Verification SCU AE Specification

4.2.1.1 SOP Classes

For SOP Classes supported, please refer to "Table 1 - Network Services" section "Verification" in chapter 1 "[Conformance Statement Overview](#)".

4.2.1.2 Association Policies

4.2.1.2.1 General

The syngo DICOM Service Tool application attempts to open an association for verification request whenever the "verification" function is activated during network configuration of a remote DICOM application.

4.2.1.2.2 Number of Associations

The syngo DICOM Service Tool application initiates one association at a time to request verification.

4.2.1.2.3 Asynchronous Nature

The syngo DICOM software does not support asynchronous communication (multiple outstanding transactions over a single association).

4.2.1.2.4 Implementation Identifying Information

For Implementation Identifying Information please refer to "Table 3 - Implementation Identifying Information" in chapter 1 "[Conformance Statement Overview](#)".

4.2.1.3 Association Initiation Policy

4.2.1.3.1 Activity – "Verification"

4.2.1.3.1.1 Description and Sequencing of Activity

The Verification SCU C-ECHO request is initiated by Service and Configuration SW whenever "Verification" is requested. If an association to a remote Application Entity is successfully established, Verification with the configured AET is requested via the open association. If the C-ECHO Response from the remote Application contains a status other than "Success" this will be indicated in the service environment and the association is closed.

4.2.1.3.1.2 Proposed Presentation Contexts

The syngo DICOM application will propose Presentation Contexts as shown in the following table:

Table 4 - Presentation Context Table "Verification"

Presentation Context Table – "Verification"					
Abstract Syntax		Transfer Syntax		Role	Extended Negotiation
Name	UID	Name List	UID List		
Verification	1.2.840.10008.1.1	Explicit VR Little Endian	1.2.840.10008.1.2.1	SCU	None
		Implicit VR Little Endian	1.2.840.10008.1.2		
		Explicit VR Big Endian	1.2.840.10008.1.2.2		

4.2.1.3.1.3 SOP Specific Conformance – Verification SCU

The Application conforms to the definition of the Verification SCU in accordance to the DICOM Standard.

4.2.1.4 Association Acceptance Policy

The Verification SCP is part of the Storage SCP.

4.2.2 Storage SCU AE Specification

4.2.2.1 SOP Classes

For SOP Classes supported, please refer to “Table 1 - Network Services”, sections “Transfer” and “Workflow Management”.

4.2.2.2 Association Policies

4.2.2.2.1 General

The DICOM Storage application will be triggered by the transfer job queue or by an external retrieve request. An association request is sent to the destination AE and, upon successful negotiation of a Presentation Context, the transfer is started. Depending on configuration, processing or resizing can be applied to the images prior to being sent.

With a Send Job successfully completed, the syngo DICOM application will generate the Storage Commitment Action Information which references to all Instances of the processed job. The Commit Request is sent over a single opened association. The syngo will wait for Status responses of the Storage Commitment Request. If the Provider accepts the Storage Commitment with Success Status, the generated Transaction UID, together with study identification data and a time-stamp, is kept. Depending on configuration, the association is closed or kept open for a configured time range. If the association is closed immediately, the response is expected on a different association which is the default setting. Multiple Storage Commitment Requests can be pending.

The default PDU size from syngo will be 515KB.

4.2.2.2.2 Number of Associations

The syngo DICOM application initiates several associations at a time, one for each destination to which a transfer request is being processed in the active job queue list.

The number of simultaneous DICOM associations can be configured via the Service-UI. The dialog can be found in "Configuration / DICOM / General".

4.2.2.2.3 Asynchronous Nature

The syngo DICOM software supports asynchronous communication (multiple outstanding transactions over a single association).

syngo supports sending/receiving of the DICOM objects in asynchronous mode during network transfers. The asynchronous mode allows the user to specify a window size i.e Max Operations Invoked and Max Operations Performed for both SCU and SCP. The window size defines, the number of request messages can be sent/received over an association before a response message is required to be received.

Note: As this is optional configuration, the asynchronous communication configuration features can be enabled through the service UI in Configuration / DICOM / General for the local machine, and in DICOM/Network Nodes page for Remote machines.

4.2.2.2.4 Implementation Identifying Information

For Implementation Identifying Information please refer to “Table 3 - Implementation Identifying Information” in chapter 1 “[Conformance Statement Overview](#)”.

4.2.2.3 Association Initiation Policy

If a job with network destination gets active in the job list or a retrieve sub-operation is processed, the syngo DICOM application attempts to initiate a new association for

- DIMSE C-STORE to send images and with successful status and
- N-ACTION DIMSE for the Storage Commitment Push Model Service Class to request commitment.

4.2.2.3.1 Activity – “Send to ...”

4.2.2.3.1.1 Description and Sequencing of Activity

The C-STORE request is triggered by a job with network destination or the processing of an external C-MOVE retrieve request. If the process successfully establishes an association to a remote Application Entity, it will transfer each image one after another via the open association. Processing features and resizing of the pixel matrix can be applied as part of the transfer. If the C-STORE Response from the remote Application contains a status other than “Success” or “Warning”, the association is aborted.

With success status for the previous transfer, the syngo Storage application sends the commit request (N-ACTION-RQ) message and waits for acceptance of this request (N-ACTION-RSP). After receiving this, the transaction is marked as “waiting”.

Depending on a configuration value, the association will then be closed or kept open. In the first case, there is another configurable timeout giving the number of hours (h) and minutes (m) (by default 1h:0m) to wait for the corresponding commit response (N-EVENT-REPORT). In the second case, this time is the (also configurable) time-out for the association being kept open. In both cases, if the commit response (N-EVENT-REPORT) does not arrive within the configured time-out, the transaction will be marked as failed.

If the commit response (N-EVENT-REPORT) received has the status of “complete - failure exists”, the transaction is marked as failed, else the transaction is marked as “completed”. In both cases, a status message is shown to the user.

4.2.2.3.1.2 Proposed Presentation Contexts

The syngo DICOM application will propose Storage SCU Presentation Contexts as shown in the following table. Kindly refer Table 1 in chapter 1 “[Conformance Statement Overview](#)”.

Table 5 - Presentation Context Table “Send to ...”

Presentation Context Table – “Send to ...”				
Abstract Syntax	Transfer Syntax		Role	Ext. Neg.
Description	Name List	UID List		
Any image SOP Class detailed in “Table 1 - Network Services” section „Transfer (Image SOP Class)“.	JPEG Lossy Extended *1	1.2.840.10008.1.2.4.51	SCU	None
	JPEG Lossless, Process 14 (selection value 1)	1.2.840.10008.1.2.4.70		
	JPEG Lossy Baseline (Process 1) *1	1.2.840.10008.1.2.4.50		
	Explicit VR Little Endian	1.2.840.10008.1.2.1		
	Explicit VR Big Endian	1.2.840.10008.1.2.2		
	Implicit VR Little Endian	1.2.840.10008.1.2		
	RLE *2	1.2.840.10008.1.2.5		
JPEG LS LOSSLESS *2	1.2.840.10008.1.2.4.80			
Any Non-image SOP Class detailed in “Table 1 - Network Services” section „Transfer (Non-image SOP Class)“.	Explicit VR Little Endian	1.2.840.10008.1.2.1	SCU	None
	Explicit VR Big Endian	1.2.840.10008.1.2.2		
	Implicit VR Little Endian	1.2.840.10008.1.2		
Private SOP Class as detailed in Chapter “Table 1 - Network Services” section „Transfer (Private SOP Class)“.	Explicit VR Little Endian	1.2.840.10008.1.2.1	SCU	None
	Explicit VR Big Endian	1.2.840.10008.1.2.2		
	Implicit VR Little Endian	1.2.840.10008.1.2		
Storage Commitment SOP Class as	Explicit VR Little Endian	1.2.840.10008.1.2.1	SCU	None

Presentation Context Table – “Send to ...”				
Abstract Syntax	Transfer Syntax		Role	Ext. Neg.
Description	Name List	UID List		
detailed in “Table 1 - Network Services” section “Workflow Management”.	Explicit VR Big Endian Implicit VR Little Endian	1.2.840.10008.1.2.2 1.2.840.10008.1.2		

*1: The Transfer Syntax used is strongly influenced by the fact of “how was the accepted Transfer Syntax at the time when the Instance was received”. e.g. the Instances received with JPEG Lossy Transfer Syntaxes will not be converted and can only be sent out with the same Transfer Syntax.

*2: During transfer of ‘X-Ray 3D Angiographic Image Storage’ which has IMAGE Type tag (0008, 0008) value contains ‘4D_DSA’ and transfer of syntax of the sending images are RLE or JPEG LS LOSSLESS, then the sending images are sent as it is without modification in the PIXEL data.

Note:

1. The proposed Transfer Syntax is highly restricted for images stored internally in lossy compressed format. E.g. instances received with JPEG Loss Transfer Syntaxes will not be converted and can only be sent out with the same Transfer Syntax.

2. The compression is only supported for images with pixel representation (0028, 0103) equal to 0 (=unsigned)

The “MOVE destinations” must be configured as Storage destinations. This would include the configuration of Transfer Syntax capabilities.

Not all the listed transfer syntaxes will be proposed all the time. For some abstract syntaxes only a list of uncompressed (UC) transfer syntaxes (one or more) will be proposed, for other abstract syntaxes also JPEG Lossless (LL) syntax will be proposed and/or a list of JPEG Lossy (LY) transfer syntaxes. The contents of this lists is configurable, e.g. UC could be configured to contain only Implicit Little Endian for instance.

Depending on the real world activity initiating the C-STORE, we have the following behaviors:

- if the C-STORE is initiated by a user, a configuration parameter called QualityFactor(Q) will be used to decide which transfer syntax lists will be proposed. Q can take values between 0 and 100. If Q=0, only UC will be proposed. If Q = 100, UC and LL will be proposed. Else UC and LY will be proposed.
- if the C-STORE is initiated by the C-MOVE SCP, there is another configuration parameter called Compression Types Supported (CTS) which will be used to decide what transfer syntaxes are proposed. CTS can take integer values. If CTS=0 or CTS > 3, UC will be proposed. If CTS=1, UC and LY will be proposed. If CTS = 2, UC and LL will be proposed. If CTS >= 3, UC, LL and LY will be proposed.

The compression types JPEG lossy and JPEG lossless are parameters, which are part of the Application Entity Properties configuration (storage checked). It can be reached via the Service-UI: Configuration / DICOM / Network nodes

4.2.2.3.1.3 SOP specific Conformance - "Send to ..."

The syngo can send images in different formats. In a destination specific service level configuration it can be configured if images are sent original, resized (512x512 8 bit, 1024x1024 12 bit) and/or processed.

For association and DIMSE level time-outs, please refer to section [Configuration](#) (4.4.2 Parameters) of this document.

4.2.2.3.1.3.1 Optional Attributes

Please refer to the related Image Object definition tables in the Annex (section "[Created SOP Instances](#)") for a list of all DICOM IOD attributes of type 2 and 3, which are encoded by the syngo applications.

4.2.2.3.1.3.2 Specialized Information Object Definitions

The DICOM images sent by syngo DICOM application conform to the DICOM IOD definitions (Standard extended IODs). But they will contain additional private elements, which have to be discarded by a DICOM system when modifying the image.

The DICOM nodes are responsible for data consistency when modifying images. All unknown private attributes have to be removed upon modification!

4.2.2.3.1.3.3 Data Dictionary of applied private IOD Attributes

Please refer to "[Standard Extended/Specialized/Private SOP Classes](#)" in the Annex for a list of possible private IOD attributes.

4.2.2.3.1.4 SOP specific Conformance - Request Commitment

Storage Commitment is supported for all the SOP Classes detailed in Chapter "Table 1 - Network Services" section "Workflow Management".

The Referenced Study Component Sequence is not supported.

Storage Media File-Set ID and UID Attributes will not be supported in the commitment request (N-ACTION primitive) invoked by the Storage Commitment SCU.

4.2.2.4 Association Acceptance Policy

4.2.2.4.1 Activity – Update Flag Information

4.2.2.4.1.1 Description and Sequencing of Activity

After sending a Storage Commitment Request the syngo either waits on the same association or, being configured to receive response on a separate association, closes the association and waits for an association request from the Storage Commitment SCP that wants to send the results.

Any incoming Notification will be checked for validity, that is, if the related Transaction UID is still part of the Pending Request Queue.

If the Notification is valid the related Instances are marked with the reported status. The over-all Commit Status of the higher Information Entities in the syngo database is derived from propagation of the States of all sub-ordinate Image entities included in a study.

The Status Flags directly affected by Storage Commitment results and indicated in the different entities of the Patient Browser list can be one of

- “AC” or “SC” - Successful Commitment, "A" means archived to configured Archive destination, whereas "S" means sent to any other destination.
- “Af” or “Sf” - Commitment failed.
- “A?” or “S?” - Commitment request is sent, response is pending.

In case of failure the user has to repeat the transfer of images to the Archive destination. Another Storage Commitment will be performed after sending is completed successfully.

4.2.2.4.1.2 Accepted Presentation Context

The syngo DICOM application will accept Storage Commitment Presentation Contexts as shown in the following table:

Table 6 - Presentation Context Table "Update Flag Information"

Presentation Context Table – “Update Flag Information”				
Abstract Syntax	Transfer Syntax		Role	Ext. Neg.
Description	Name List	UID List		
1.2.840.10008.1.20.1 Storage Commitment Push Model	Explicit VR Little Endian Explicit VR Big Endian Implicit VR Little Endian	1.2.840.10008.1.2.1 1.2.840.10008.1.2.2 1.2.840.10008.1.2	SCP	None

4.2.2.4.1.3 SOP specific Conformance

If the Commitment response (N-EVENT-REPORT) received has the status of “complete - failure exists”, the transaction is marked as failed, else the transaction is marked as “completed”. In both cases, a message is shown to the user.

The related status flags are set for the committed images in the local database.

The syngo DICOM application will not support the Storage Media File Set ID attributes.

4.2.3 Storage SCP AE Specification

4.2.3.1 SOP Classes

For SOP Classes supported, please refer to “Table 1 - Network Services” Sections “Transfer” on page 2.

4.2.3.2 Association Policies

4.2.3.2.1 General

The syngo DICOM application will accept any number of verification or storage SOP classes that are referred to above. There is no limit on the number of presentation contexts accepted except for the DICOM limit. In the event that the Siemens DICOM application runs out of resources, it will reject the association request.

When "trusted host functionality" is enabled syngo will only accept Associations from known hosts with a known AET. Hosts and AETs have to be entered in "Local Service" by a Siemens CSE.

The default PDU size from syngo will be 515KB.

4.2.3.2.2 Number of Associations

The Siemens syngo DICOM application is able to accept multiple associations at a time. It can handle up to 10 associations in parallel.

The number of simultaneous DICOM associations can be configured via the Service-UI. The dialog can be found in "Configuration / DICOM / General".

4.2.3.2.3 Asynchronous Nature

The syngo DICOM software supports asynchronous communication (multiple outstanding transactions over a single association)

syngo supports sending/receiving of the DICOM objects in asynchronous mode during network transfers. The asynchronous mode allows the user to specify a window size i.e Max Operations Invoked and Max Operations Performed for both SCU and SCP. The window size defines, the number of request messages can be sent/received over an association before a response message is required to be received.

Note: As this is optional configuration, the asynchronous communication configuration features can be enabled through the service UI in Configuration / DICOM / General for the local machine, and in DICOM/Network Nodes page for Remote machines.

4.2.3.2.4 Implementation Identifying Information

For Implementation Identifying Information please refer to “Table 3 - Implementation Identifying Information” in chapter 1 [“Conformance Statement Overview”](#).

4.2.3.3 Association Initiation Policy

If the result from a previously accepted Storage Commitment request is evaluated, the syngo DICOM application attempts to initiate a new association for

- DIMSE N-EVENT-REPORT for sending commitment result from a previous request.

4.2.3.3.1 Activity - Return Commitment Result

When syngo Storage SCP AE received a Storage Commitment request it tries to send the response back on the same association. When the association is not open anymore it will initiate an association to send the Storage Commitment response (N-EVENT-REPORT) to the SCU.

4.2.3.3.1.1 Proposed Presentation Context

The syngo DICOM application will propose Storage SCP Presentation Contexts for returning Storage Commitment results as shown in the following table:

Table 7 - Presentation Context Table "Return Commitment Result"

Presentation Context Table – "Return Commitment Result"				
Abstract Syntax	Transfer Syntax		Role	Ext. Neg.
Description	Name List	UID List		
Storage Commitment SOP Class as detailed in "Table 1 - Network Services" section "Workflow Management".	Explicit VR Little Endian	1.2.840.10008.1.2.1	SCP	None
	Explicit VR Big Endian	1.2.840.10008.1.2.2		
	Implicit VR Little Endian	1.2.840.10008.1.2		

4.2.3.3.1.2 SOP Specific Conformance

Storage Media File-Set ID and UID Attributes will not be supported in the N-EVENT-REPORT primitive invoked by the Storage SCP.

4.2.3.4 Association Acceptance Policy

The syngo DICOM application attempts to accept a new association for

- DIMSE C-ECHO for incoming Verification requests
- DIMSE C-STORE for external image senders request storage of instances
- DIMSE N-ACTION for external systems requesting Storage Commitment
- DIMSE N-EVENT-REPORT for receiving commitment result from a previous request

4.2.3.4.1 Activity – Save to local disk

4.2.3.4.1.1 Description and Sequencing of Activity

The syngo DICOM application will accept an association and will receive SOP Instances according to the listed presentation contexts on that association and will store the images to the local hard disk if the conformance check is performed successfully.

Upon successful receiving a C-STORE-RQ, the syngo DICOM receiver performs a plausibility test on the received image and available system resources. If this test succeeds, it returns the Status SUCCESS, otherwise one of the following status codes is returned and the association is aborted:

Table 8 - Status codes "Save to local disk"

Code	Meaning
A700	<u>Refused</u> : This error status indicates a lack of Resources (e.g. not enough disk space) on the syngo modality.
A900	<u>Invalid Dataset</u> : An error occurred while processing the image, which makes it impossible to proceed. The image will not be stored and the association is aborted.
0110	<u>Processing Error</u> : An error occurred while processing the image, which makes it impossible to proceed. Association is aborted.

Note: The image will be saved after sending the response. If during this operation an error occurs, the association will be aborted. This implies that a C-STORE-RSP with status SUCCESS does not mean that the image was successfully stored into the database.

4.2.3.4.1.2 Accepted Presentation Context

The syngo DICOM application will accept Presentation Contexts as shown in the following table. . Kindly refer Table 1 in Chapter 1 [“Conformance Statement Overview”](#) for details.

Table 9 - Presentation Context Table "Save to local disk"

Presentation Context Table – “Save to local disk”				
Abstract Syntax	Transfer Syntax		Role	Ext. Neg.
Description	Name List	UID List		
Any image SOP Class detailed in “Table 1 - Network Services” section „Transfer (Image SOP Class)“.	JPEG Lossy Extended (Process 2 & 4)	1.2.840.10008.1.2.4.51	SCP	None
	JPEG Lossless, Process 14 (selection value 1)	1.2.840.10008.1.2.4.70		
	JPEG Lossless, Process 14, Non-HIER	1.2.840.10008.1.2.4.57		
	JPEG Lossy Baseline (Process 1)	1.2.840.10008.1.2.4.50		
	RLE Lossless	1.2.840.10008.1.2.5		
	Explicit VR Little Endian	1.2.840.10008.1.2.1		
	Explicit VR Big Endian	1.2.840.10008.1.2.2		
	Implicit VR Little Endian	1.2.840.10008.1.2		
	JPEG 2000 Lossless	1.2.840.10008.1.2.4.90		
	JPEG 2000 Lossy	1.2.840.10008.1.2.4.91		
	JPEG LS LOSSLESS	1.2.840.10008.1.2.4.80		
Any non-image SOP Class detailed in “Table 1 - Network Services” section „Transfer (Non-image SOP Class)“.	Explicit VR Little Endian	1.2.840.10008.1.2.1	SCP	None
	Explicit VR Big Endian	1.2.840.10008.1.2.2		
	Implicit VR Little Endian	1.2.840.10008.1.2		
Private SOP Class as detailed in Chapter “Table 1 - Network Services” section „Transfer (Private SOP Class)“.	Explicit VR Little Endian	1.2.840.10008.1.2.1	SCP	None
	Explicit VR Big Endian	1.2.840.10008.1.2.2		
	Implicit VR Little Endian	1.2.840.10008.1.2		

Note:

- 1.US Image Storage and US Multiframe Image Storage are converted to US Images/US Multi-frame images before storing them into the local database. The conversion creates new images, which implies new UIDs.
- 2.With RLE Lossless Transfer Syntax and JPEG Lossless, Process 14, Non-HIER Transfer Syntax the DICOM application will decompress the image before storing it into the database.
- 3.JPEG 2000 decompression supported only for import in connection with COSMOS workplace.
- 4.Private attributes in sequence items will be removed during import into syngo.
- 5.Receiving of Enhanced CT and Enhanced MR images with concatenated data is not supported. This is realized by checking the Concatenation UID (Tag ID: 0020, 9161) of Multi-Frame Functional Group, which will be set for Concatenated data.
- 6.After receiving the images of type Multi-frame Single Bit Secondary Capture Image, Multi-frame Grayscale Byte Secondary Capture Image, Multi-frame Grayscale Word Secondary Capture Image and Multi-frame True Color Secondary Capture Image, the SOP class UID of received image is changed and stored as Secondary Capture Image (1.2.840.10008.5.1.4.1.1.7). The SOP Class UID will be stored as private attribute and while sending it SOP Class UID will be updated back to original.
7. During receiving of the images ‘X-Ray 3D Angiographic Image Storage’ which has IMAGE Type tag (0008, 0008) value contains ‘4D_DSA’ and transfer of syntax of the received images are RLE or JPEG LS LOSSLESS, then the received images are stored as it. The received images are not decompressed.

4.2.3.4.1.3 SOP specific Conformance

The syngo application conforms to the Full Storage Service Class at Level 2.

Any Explicit VR Transfer Syntax is preferred to be used by the Storage SCU when sending Composite Image Instances to the syngo DICOM application.

If an image instance is received that is identified by a SOP Instance UID which is already used by an Instance stored in database then the actual received image will be discarded. The existing Instance is not superseded.

The order of preference in accepting Transfer Syntaxes within Presentation Contexts or Presentation Contexts with single Transfer Syntaxes is:

Table 10 - Order of Preference Transfer Syntax

Order	DICOM Transfer Syntax
1	JPEG Lossy Extended
2	JPEG Lossless hierarchical
3	JPEG Lossy Baseline
4	RLE Lossless
5	Explicit VR Little Endian
6	Explicit VR Big Endian
7	Implicit VR Little Endian
8	JPEG 2000 Lossy
9	JPEG 2000 Lossless
10	JPEG Lossless Non-hierarchical
11	JPEG LS LOSSLESS

With RLE Lossless, JPEG 2000 Lossy and JPEG 2000 Lossless Transfer Syntax the syngo DICOM application will decompress the image before storing it into the database.

With Implicit VR Little Endian Transfer Syntax the syngo DICOM application will remove any Private Attributes not known to the application. Decision on removal of a Private Element is done if there is NO entry in the attribute-dictionary of the syngo DICOM application.

Therefore any Explicit VR Transfer Syntax shall preferably be used by the Storage SCU's when sending Composite Image Instances to the syngo DICOM application.

The following sections will differentiate the attribute contents required for Image Viewing. The syngo DICOM application supports more formats for Storage of Images than for Viewing.

Image Pixel Attribute Acceptance Criterion for Grayscale Images

The syngo Multi-Modality Viewing application accepts the MONOCHROME1 and MONOCHROME2 photometric interpretation pixel format and graphic overlay with unsigned integer and 8 or 16 bits allocated. Accepted values:

Pixel plane

- samples per pixel (attribute 0028, 0002) = 1
- photometric interpretation (attribute 0028,0004) = "MONOCHROME1"
- photometric interpretation (attribute 0028,0004) = "MONOCHROME2"
- pixel representation (attribute 0028, 0103) = 0
- bits allocated (attribute 0028, 0100) = 8, 16
- bits stored (attribute 0028,0101) = 8, 10, 12, 14, 15, 16
- high bit (attribute 0028,0102) = 7, 9, 11
- only aspect ratio 1:1 is supported

Overlay plane

- overlay type (attribute 60xx, 0040) = "G"
- bits allocated (attribute 60xx, 0100) = 16
- bit position (attribute 60xx, 0102) = 12, 13, 14, 15 (only bits above high bit permitted)
- Graphic Overlay will be shifted to fill Overlay Planes from Bit 12 and consecutive.

Overlay plane

- Overlay Type (60xx,0040) = "G"
- Bits Allocated (60xx,0100) = 1
- Bit Position (60xx,0102) = 0
- Overlay Data (60xx,3000) = supported

The syngo Multi-Modality Viewing application accepts also the MONOCHROME1 and MONOCHROME2 photometric interpretation pixel format with binary 2's complement integer and 16 bits allocated. Accepted values:

Pixel plane

- samples per pixel (attribute 0028, 0002) = 1
- photometric interpretation (attribute 0028,0004) = "MONOCHROME1"
- photometric interpretation (attribute 0028,0004) = "MONOCHROME2"
- pixel representation (attribute 0028, 0103) = 1 (signed)
- bits allocated (attribute 0028, 0100) = 16
- bits stored (attribute 0028,0101) = 16
- high bit (attribute 0028,0102) = 15
- only aspect ratio 1:1 is supported

Overlay plane

- overlay type (attribute 60xx, 0040) = "G"
- bits allocated (attribute 60xx, 0100) = 1
- bit position (attribute 60xx, 0102) = 0
- overlay data (attribute 60xx, 3000) = supported
- For MOD LUT, both the linear LUT (Rescale Slope/Intercept) and the MOD LUT SQ are supported and considered when pixel data is displayed. However there are two limitations. The MOD LUT SQ will be ignored in the following cases:
 - 8-Bit signed pixels
 - the pixel format is changed by the MOD LUT (e.g. 8bit -> 16bit)

If the MOD LUT SQ contains multiple LUTs, then only the first one is used.

For VOI LUT, both the linear LUT (Window Center/Width) and the VOI LUT SQ are supported (VOI LUT SQ with 8 or 16 bit LUT data)

But if both, a VOI LUT SQ and a linear MOD LUT, are specified within one image, then the value for Rescale Slope is restricted to 1.

If the VOI LUT SQ contains multiple LUTs, then only the first one is used by default. The other VOI LUTs are selectable.

Only Rectangular and Circular Shutter Shape is supported in this version. Images containing other Shutter Shapes will be displayed w/o shutter.

Image Pixel Attribute Acceptance Criterion for Color Images Viewing

The syngo Multi-Modality Viewing application supports the RGB color image description with the unsigned integer 24-bit color image plane pixel format.

Accepted values:

- samples per pixel (attribute 0028, 0002) = 3
- photometric interpretation (attribute 0028,0004) = "RGB"
- pixel representation (attribute 0028, 0103) = 0
- bits allocated (attribute 0028, 0100) = 8
- bits stored (attribute 0028,0101) = 8
- high bit (attribute 0028,0102) = 7
- planar configuration (attribute 0028,0006) = 0 (pixel interleave) or 1 (plane interleave).

The syngo Multi-modality Viewing application supports the "Palette Color" color image description with the unsigned integer and 2's complement pixel format. Accepted values:

- samples per pixel (attribute 0028, 0002) = 1
- photometric interpretation (attribute 0028,0004) = "PALETTE COLOR"
- pixel representation (attribute 0028, 0103) = 0
- bits allocated (attribute 0028, 0100) = 8 and bits stored (attribute 0028,0101) = 8
- bits allocated (attribute 0028, 0100) = 16 and bits stored (attribute 0028,0101) = 16
- high bit (attribute 0028,0102) = 7, 15
- Both 8-bit and 16-bit palettes are supported, but NO Segmented Palette Color LUTs.

The syngo Multi-modality Viewing application supports the YBR color image description with the unsigned integer pixel format. Accepted values:

- samples per pixel (attribute 0028, 0002) = 3
- photometric interpretation (attribute 0028,0004) = "YBR_FULL" or "YBR_FULL_422"
- pixel representation (attribute 0028, 0103) = 0
- bits allocated (attribute 0028, 0100) = 8 and bits stored (attribute 0028,0101) = 8
- high bit (attribute 0028,0102) = 7

If syngo software is making any persistent changes on a YBR image, the resulting new image will be saved with Photometric Interpretation = "RGB".

4.2.3.4.2 Activity – Evaluate Commit Request

4.2.3.4.2.1 Description and Sequencing of Activity

When receiving a Storage Commitment request the syngo DICOM application will perform the necessary steps to check the received list Instances against the local database.

4.2.3.4.2.2 Accepted Presentation Context

The syngo DICOM application will accept Storage Commitment Presentation Contexts as shown in the following table:

Table 11 - Presentation Context Table "Evaluate Commit Request"

Presentation Context Table – "Evaluate Commit Request"				
Abstract Syntax	Transfer Syntax		Role	Ext. Neg.
Description	Name List	UID List		
Storage Commitment SOP Class detailed in "Table 1 - Network Services" section "Workflow Management".	Explicit VR Little Endian	1.2.840.10008.1.2.1	SCP	None
	Explicit VR Big Endian	1.2.840.10008.1.2.2		
	Implicit VR Little Endian	1.2.840.10008.1.2		

4.2.3.4.2.3 SOP specific Conformance

The syngo Storage SCP AE will return success for images that are stored in the local database and failure for images that are not. However, the committed images can later be deleted by the user at the syngo without notice!

Note: Storage Media File-Set ID and UID Attributes will not be supported in the N-EVENT-REPORT primitive invoked by the Storage Commitment SCP.

4.2.4 Query/Retrieve SCU Specification

4.2.4.1 SOP Classes

For SOP Classes supported, please refer to “Table 1 - Network Services” section „Query/Retrieve“ in chapter 1 [“Conformance Statement Overview”](#).

4.2.4.2 Association Policies

4.2.4.2.1 General

With the "Search..." function the query data can be entered and the DICOM Query/Retrieve application is initiated. An initial query request will be sent out to one remote node that can be selected from a list of configured Query Providers. Depending on the replies to the initial request, subsequent query requests are issued to gather further data for lower information level entities. The results compiled from the response data will be displayed to the user. Upon request (Import), the retrieval of selected items is initiated.

The default PDU size from syngo will be 515KB.

4.2.4.2.2 Number of Associations

The syngo DICOM application initiates several associations at a time.

For Query it initiates a new association to the remote node and issues the C-FIND request to retrieve all the requested patient and study information matching the search criteria. All the subsequent calls for C-FIND to obtain information on sub-studies and sub-series run in parallel i.e. multiple associations are being initiated to the remote node for C-FIND requests.

For the Retrieve request (C-MOVE) only one association is initiated per destination.

4.2.4.2.3 Asynchronous Nature

The syngo DICOM software does not support asynchronous communication (multiple outstanding transactions over a single association).

4.2.4.2.4 Implementation Identifying Information

For Implementation Identifying Information please refer to “Table 3 - Implementation Identifying Information” in chapter 1 [“Conformance Statement Overview”](#).

4.2.4.3 Association Initiation Policy

The syngo DICOM application will request associations for the following DIMSE-C operations as SCU:

Table 12 - Supported DIMSE-C Operations - Query/Retrieve SCU

Supported DIMSE operations	Cancel Request supported
C-FIND	yes
C-MOVE	n. a.

Extended negotiation (relational query) is not supported for the above listed services.

4.2.4.3.1 Activity – Search for images (Search...)

4.2.4.3.1.1 Description and Sequencing of Activity

The associated activity is to fill out a query form with search data and pass it as query to the network application which issues a C-FIND over a previously built association. The remote SCP will respond with related data-entries that will be passed to a browser application. If needed, further

associations are opened for querying data from sub-sequent entities. When data transfer is finished, each association is closed.

If the C-FIND Response from the remote Application contains an error status, the association is aborted.

4.2.4.3.1.2 Proposed Presentation Contexts

The syngo DICOM application will propose Presentation Contexts as shown in the following table:

Table 13 - Presentation Context Table "Search..."

Presentation Context Table - "Search..."					
Abstract Syntax		Transfer Syntax		Role	Ext. Neg.
Name	UID	Name List	UID List		
Patient Root Query/Retrieve Model - FIND	1.2.840.10008.5.1.4.1.2.1.1	Implicit VR Little Endian	1.2.840.10008.1.2	SCU	None
		Explicit VR Big Endian	1.2.840.10008.1.2.2		
		Explicit VR Little Endian	1.2.840.10008.1.2.1		
Study Root Query/Retrieve Model - FIND	1.2.840.10008.5.1.4.1.2.2.1	Implicit VR Little Endian	1.2.840.10008.1.2	SCU	None
		Explicit VR Big Endian	1.2.840.10008.1.2.2		
		Explicit VR Little Endian	1.2.840.10008.1.2.1		
Patient/Study Only Query/Retrieve Model - FIND	1.2.840.10008.5.1.4.1.2.3.1	Implicit VR Little Endian	1.2.840.10008.1.2	SCU	None
		Explicit VR Big Endian	1.2.840.10008.1.2.2		
		Explicit VR Little Endian	1.2.840.10008.1.2.1		

Within the DICOM network configuration it is configurable which of the two query models (or both) are to be used by the syngo DICOM Query SCU application for each node. If both Abstract Syntaxes are configured, the Find SCU will use the Patient Root Model only for C-FIND requests on PATIENT level. For all other levels it will use the Study Root model.

4.2.4.3.1.3 SOP Specific Conformance

The syngo DICOM Query/Retrieve SCU supports hierarchical queries with all mandatory search keys. The interactive querying of attributes on IMAGE level is not supported by the Query SCU, hence retrieval of individual Objects is possible. The following table describes the search keys for the different query models that the SCU supports. Matching is either wildcard, which means that the user can supply a string containing wildcards, or universal, which means that the attribute is requested as return value.

Table 14 - C-FIND RQ Search Keys

Attribute Name	Tag	Type	Matching	User Input	Return Display	Value
Patient Level^c						
Patient Name	(0010,0010)	R	Wildcard ^d	Enter value	yes	
Patient ID	(0010,0020)	U / R	Wildcard ^d	Enter value	yes	
Patient's Birth Date	(0010,0030)	O	Single value	Enter value	yes	
Patient's Sex	(0010,0040)	O	Single value	Enter value	yes	
Number of Patient related Studies	(0020,1200)	O	Universal(Null)	--	yes ^e	
Number of Patient related Series	(0020,1202)	O	Universal(Null)	--	no	
Number of Patient related Instances	(0020,1204)	O	Universal(Null)	--	no	
Study Level						
Patient Name ^f	(0010,0010)	R	Wildcard ^d	Enter value	yes	
Patient ID	(0010,0020)	U / R	Wildcard ^d	Enter value	yes	
Patient's Birth Date ^f	(0010,0030)	O	Single value	Enter value	yes	
Patient's Sex ^f	(0010,0040)	O	Single value	Enter value	yes	
Study Instance UID	(0020,000D)	U	Single value	Enter value	yes	
Study ID	(0020,0010)	R	Wildcard ^d	Enter value	yes	
Study Date	(0008,0020)	R	Range	Enter value	yes	
Study Time	(0008,0030)	R	Range	Enter value	yes	
Accession Number	(0008,0050)	R	Wildcard	Enter value	yes	
Study Description	(0008,1030)	O	Wildcard ^d	Enter value	yes	
Referring Physician's Name	(0008,0090)	O	Wildcard ^d	Enter value	yes	
Name of Physician Reading Study	(0008,1060)	O	Wildcard ^d	Enter value	yes	
Modalities in Study	(0008,0061)	O	Single Value	Enter value	yes	
Number of Patient related Studies	(0020,1200)	O	Universal(Null)	--	no	
Number of Patient related Series	(0020,1202)	O	Universal(Null)	--	no	
Number of Patient related Instances	(0020,1204)	O	Universal(Null)	--	no	
Number of Study related Series	(0020,1206)	O	Universal(Null)	--	yes ^g	

^c Patient Root Information Model only^d Always a "*" is appended to the user-supplied string^e Implicitly visualized in the UI if no study and series search attributes have been entered^f Study Root Information Model only

Attribute Name	Tag	Type	Matching	User Input	Return Display	Value
Number of Study related Instances	(0020,1208)	O	Universal(Null)	--	no	
Series Level						
Series Instance UID	(0020,000E)	U	Single Value	Enter value	yes	
Series Number	(0020,0011)	R	Single Value	Enter value	yes	
Modality	(0008,0060)	R	Single Value	Enter value	yes	
Series Date	(0008,0021)	O	Universal(Null)	--	yes	
Series Time	(0008,0031)	O	Universal(Null)	--	yes	
Series Description	(0008,103E)	O	Wildcard ^d	Enter value	yes	
Body Part Examined	(0018,0015)	O	Single Value	Enter value	yes	
Performing Physician's Name	(0008,1050)	O	Wildcard ^d	Enter value	yes	
Request Attributes Sequence	(0040,0275)	O	--	--	yes	
>Requested Procedure ID	(0040,1001)	O	Wildcard ^d	Enter value	yes	
>Scheduled Procedure Step ID	(0040,0009)	O	Wildcard ^d	Enter value	yes	
Performed Procedure Step Start Date	(0040,0244)	O	Range	Enter value	yes	
Performed Procedure Step Start Time	(0040,0245)	O	Range	Enter value	yes	
Number of Series related Instances	(0020,1209)	O	Universal(Null)	--	yes	
Instance Availability	(0008,0056)	O	Universal(Null)			
Image Level						
SOP Instance UID	(0008,0018)	U	Single Value	--	no	
Instance Number	(0020,0013)	R	Universal(Null)	--	yes	
SOP Class UID	(0008,0016)	O	Universal(Null)	--	no	
Image Comments	(0020,4000)	O	Universal(Null)	--	yes	
Number of Frames	(0028,0008)	O	Universal(Null)	--	yes	
Content Date	(0008,0023)	O	Universal(Null)	--	yes	
Content Time	(0008,0033)	O	Universal(Null)	--	yes	

U = Unique Key, **R** = Required Key, **O** = Optional Key, - = not supported or applicable

The syngo Search application supports a

- DIMSE C-FIND-CANCEL

if the user wishes to cancel a running Query request via the syngo user interface ("Cancel" button while a "Search..." is active).

The Find SCU interprets following status codes:

⁹ Implicitly if no series search attributes have been entered

Table 15 - Status Codes "Search..."

Service Status	Meaning	Error Codes	Related Fields
Refused	Out of Resources	A700	(0000,0902)
Failed	Identifier does not match SOP Class	A900	(0000,0901) (0000,0902)
	Unable to process	Cxxx	(0000,0901) (0000,0902)
Cancel	Matching terminated due to Cancel request	FE00	None
Success	Matching is complete - No final Identifier is supplied	0000	None
Pending	Matches are continuing - Current Match is supplied and any Optional Keys were supported in the same manner as Required Keys	FF00	Identifier
	Matches are continuing - Warning that one or more Optional Keys were not supported for existence and/or matching for this identifier	FF01	Identifier

4.2.4.3.2 Activity – Retrieve Images (Import...)

4.2.4.3.2.1 Description and Sequencing of Activity

When selecting a data entry in the Query UI and activating the "Import" function, a retrieval request is passed to the syngo DICOM application which issues a C-MOVE service according to the Patient Root or Study Root query model. (The Storage Service Class Conformance Statement describes the C-STORE service, which is generated by processing the C-MOVE service.)

The received image data are processed as described in the Storage class SCP descriptions.

The syngo DICOM application will always insert the own Storage SCP AE as "Move Destination".

4.2.4.3.2.2 Proposed Presentation Contexts

The syngo Server DICOM application will propose Presentation Contexts as shown in the following table:

Table 16 - Presentation Context Table "Import..."

Presentation Context Table					
Abstract Syntax		Transfer Syntax		Role	Ext. Neg.
Name	UID	Name List	UID List		
Query/Retrieve Model Patient Root – MOVE	1.2.840.10008.5.1.4.1.2.1.2	Implicit VR Little Endian Explicit VR Big Endian Explicit VR Little Endian	1.2.840.10008.1.2 1.2.840.10008.1.2.2 1.2.840.10008.1.2.1	SCU	None
Query/Retrieve Model Study Root – MOVE	1.2.840.10008.5.1.4.1.2.2.2	Implicit VR Little Endian Explicit VR Big Endian Explicit VR Little Endian	1.2.840.10008.1.2 1.2.840.10008.1.2.2 1.2.840.10008.1.2.1	SCU	None
Query/Retrieve Model Patient/Study Only – MOVE	1.2.840.10008.5.1.4.1.2.3.2	Implicit VR Little Endian Explicit VR Big Endian Explicit VR Little Endian	1.2.840.10008.1.2 1.2.840.10008.1.2.2 1.2.840.10008.1.2.1	SCU	None

Note: C-MOVE Extended Negotiation will not be supported by the SCU.

4.2.4.3.2.3 SOP Specific Conformance

All required keys will be provided in the retrieve request identifier, as defined in DICOM Standard.

The Move SCU interprets following status codes:

Table 17 - C-MOVE RSP Status Codes

Service Status	Meaning	Error Codes	Related Fields
Refused	Out of Resources - Unable to calculate number of matches	A701	(0000,0902)
	Out of Resources - Unable to perform sub operations	A702	(0000,1020) (0000,1021) (0000,1022) (0000,1023)
	Move destination unknown	A801	(0000,0902)
Failed	Identifier does not match SOP Class	A900	(0000,0901) (0000,0902)
	Unable to process	Cxxx	(0000,0901) (0000,0902)
Cancel	Sub-operations terminated due to Cancel Indication	FE00	(0000,1020) (0000,1021) (0000,1022) (0000,1023)
Warning	Sub-operations Complete - One or more Failures of Warnings	B000	(0000,1020) (0000,1021) (0000,1022) (0000,1023)
Success	Sub-operations Complete - No Failures or Warning	0000	(0000,1020) (0000,1021) (0000,1022) (0000,1023)
Pending	Sub-operations are continuing	FF00	(0000,1020) (0000,1021) (0000,1022) (0000,1023)

4.2.4.4 Association Acceptance Policy

See next section "Query/Retrieve SCP AE Specification".

4.2.5 Query/Retrieve SCP Specification

4.2.5.1 SOP Classes

For SOP Classes supported, please refer to “Table 1 - Network Services” section „Query/Retrieve“ in chapter 1 [“Conformance Statement Overview”](#).

4.2.5.2 Association Policies

4.2.5.2.1 General

When "trusted host" functionality is enabled syngo will only accept Associations from known hosts with a known AET. Hosts and AETs have to be entered in "Local Service" by a Siemens CSE.

The default PDU size from syngo will be 515KB.

4.2.5.2.2 Number of Associations

The Siemens syngo DICOM application is able to accept multiple associations at a time. It can handle up to 10 associations in parallel.

The number of simultaneous DICOM associations can be configured via the Service-UI. The dialog can be found in "Configuration / DICOM / General".

4.2.5.2.3 Asynchronous Nature

The syngo DICOM software does not support asynchronous communication (multiple outstanding transactions over a single association).

4.2.5.2.4 Implementation Identifying Information

For Implementation Identifying Information please refer to “Table 3 - Implementation Identifying Information”.

4.2.5.3 Association Initiation Policy

See previous section “Query/Retrieve SCU AE Specification”.

4.2.5.4 Association Acceptance Policy

The syngo DICOM application will accept associations for the following DIMSE-C operations as SCP:

- C-FIND
- C-GET
- C-MOVE
- C-FIND-CANCEL
- C-GET-CANCEL
- C-MOVE-CANCEL

Extended negotiation - which is relational query or retrieve - is not supported for the above listed services. The syngo DICOM application does support multiple C-FIND requests over the same association, while multiple C-MOVE or C-GET operations are not supported over the same association.

4.2.5.4.1 Activity - Process Search Requests

4.2.5.4.1.1 Description and Sequencing of Activity

The Query SCP AE will respond to incoming query requests from a SCU with the query model Patient Root, Study Root and Patient/Study Only. Relational retrieve operation is not supported. The content records of the local database are used to match the incoming query keys and fill the related return keys. With a C-FIND-CANCEL request the running query can be canceled at any time.

Multiple C-FIND requests over the same association are supported.

4.2.5.4.1.2 Accepted Presentation Contexts

The syngo DICOM application will accept Presentation Contexts as shown in the following table:

Table 18 - Presentation Context Table "Process Search Requests"

Presentation Context Table					
Abstract Syntax		Transfer Syntax		Role	Ext. Neg.
Name	UID	Name List	UID List		
Patient Root Query/Retrieve Model - FIND	1.2.840.10008.5.1.4.1.2.1.1	Implicit VR Little Endian	1.2.840.10008.1.2	SCP	None
		Explicit VR Big Endian	1.2.840.10008.1.2.2		
		Explicit VR Little Endian	1.2.840.10008.1.2.1		
Study Root Query/Retrieve Model - FIND	1.2.840.10008.5.1.4.1.2.2.1	Implicit VR Little Endian	1.2.840.10008.1.2	SCP	None
		Explicit VR Big Endian	1.2.840.10008.1.2.2		
		Explicit VR Little Endian	1.2.840.10008.1.2.1		
Patient/Study Only Query/Retrieve Model - FIND	1.2.840.10008.5.1.4.1.2.3.1	Implicit VR Little Endian	1.2.840.10008.1.2	SCP	None
		Explicit VR Big Endian	1.2.840.10008.1.2.2		
		Explicit VR Little Endian	1.2.840.10008.1.2.1		

Note: C-FIND Extended Negotiation will not be supported.

The order of preference for accepting Transfer Syntaxes is: 1. Explicit VR Little Endian, 2. Explicit VR Big Endian, 3. Implicit VR Little Endian.

4.2.5.4.1.3 SOP Specific Conformance

The syngo DICOM Query/Retrieve SCP supports hierarchical queries for all mandatory and optional search keys.

The syntactical component structure of the attribute (0010,0010) Patients Name is defined as follows (see [DICOM], Part 5, Definition of PN, Person Name):

<single byte group> =<ideographic group>=<phonetic group>

The Query/Retrieve SCP replies to queries for "Patient Name" as follows:

1. Matching of Patients Name attribute (0010, 0010) is done case-insensitive.
2. If a search string matches the complete value of a Patient's Name in the database, a match will be returned.
3. If a search string matches an individual group (single byte, ideographic or phonetic) of a Patient's Name in the database, a match will be returned.

4. If a search string matches two consecutive groups of a data base object's Patients Name, a match will be returned.
5. Redundant group separators "=" or component separators "^" are treated as insignificant for matching.
6. Leading and trailing blanks within a component or a group of Patient's Name are treated as insignificant for matching.

Except for attribute Patient's Name (0010,0010) any queries for text string attributes will be treated case-sensitive.

The Find SCP will not differentiate "?" and "**", thus "?abc*" will be treated as "**abc*".

If the value for the patient-level unique key "Patient ID" is not known, it will be returned with zero length. The attribute "Image Comments" will not be included in the C-FIND-RSP, if it is not set in the DB, even if it was requested as return key in the related C-FIND-RQ.

Usage of Storage Media File-Set ID, Retrieve AE Title with C-FIND-RSP message:

- The Storage Media File-Set ID - if available - can be returned at Study/Series/Image Level. Only on Image Level, the values of ONLINE, NEARLINE or OFFLINE are returned to indicate the Storage Location of the related Instance.
- The Retrieve AE Title - if available - can only be returned at Image Level (for Patient Root and Study Root models) or Study Level (for Patient/Study Only model).

Relational Queries are not supported.

A remote DICOM AE can cancel the running query by sending a C-FIND-CANCEL. Matches are possibly continuing (more C-FIND response with status PENDING) until the cancel operation takes effect and query matching has completed.

The supported attributes on the various query levels of the three supported information models are listed in the following table.

Table 19 - Query/Retrieve SCP supported attributes

Attribute Name	Tag	PR	SR	PSo	Matching
Patient Level (PR or PSo) or Study Level (SR)					
Patient Name	(0010,0010)	R	R	R	Single value, Wildcard, universal
Patient ID	(0010,0020)	U	R	U	Single Value, Wildcard, universal
Patient's Birth Date	(0010,0030)	O	O	O	Single Value, Range, universal
Patient's Birth Time	(0010,0032)	O	O	O	Single Value, Range, universal
Patient's Sex	(0010,0040)	O	O	O	Single Value, Wildcard, universal
Ethnic Group	(0010,2160)	O	-	O	Single Value, Wildcard, universal
Patient Comments	(0010,4000)	O	O	O	Wildcard, universal
Number of Patient related Studies	(0020,1200)	O	O	O	universal
Number of Patient related Series	(0020,1202)	O	O	O	universal
Number of Patient related Instances	(0020,1204)	O	O	O	universal
Study Level					

Attribute Name	Tag	PR	SR	PSo	Matching
Study Instance UID	(0020,000D)	U	U	U	Single Value, List of UIDs
Study ID	(0020,0010)	R	R	R	Single Value, Wildcard, universal
Study Date	(0008,0020)	R	R	R	Single Value, Range, universal
Study Time	(0008,0030)	R	R	R	Single Value, Range, universal
Accession Number	(0008,0050)	R	R	R	Single Value, Wildcard, universal
Referring Physician's Name	(0008,0090)	O	O	O	Single Value, Wildcard, universal
Study Description	(0008,1030)	O	O	O	Single Value, Wildcard, universal
Admitting Diagnosis Description	(0008,1080)	O	O	O	Single Value, Wildcard, universal
Patient's Age	(0010,1010)	O	O	O	Single Value, Wildcard, universal
Patient's Size	(0010,1020)	O	O	O	Single Value, universal
Patient's Weight	(0010,1030)	O	O	O	Single Value, universal
Occupation	(0010,2180)	O	O	O	Single Value, Wildcard, universal
Additional Patient History	(0010,21B0)	O	O	O	Wildcard, universal
Name of Physician reading the Study	(0008,1060)	O	O	O	Single Value, Wildcard, universal
Modalities in Study	(0008,0061)	O	O	O	Multiple values, universal
Number of Study Related Series	(0020,1206)	O	O	O	universal
Number of Study Related Instances	(0020,1208)	O	O	O	universal
Series Level					
Series Instance UID	(0020,000E)	U	U	-	Single Value, List of UIDs
Series Number	(0020,0011)	R	R	-	Single Value, universal
Modality	(0008,0060)	R	R	-	Single Value, Wildcard, universal
Laterality	(0020,0060)	O	O	-	Single Value, Wildcard, universal
Body Part Examined	(0018,0015)	O	O	-	Single Value, Wildcard, universal
Patient Position	(0018,5100)	O	O	-	Single Value, Wildcard, universal
Smallest Pixel Value in Series	(0028,0108)	O	O	-	Single Value, universal
Largest Pixel Value in Series	(0028,0109)	O	O	-	Single Value, universal
Protocol Name	(0018,1030)	O	O	-	Single Value, Wildcard, universal
Series Date	(0008,0021)	O	O	-	Single Value, Range, universal
Series Time	(0008,0031)	O	O	-	Single Value, Range, universal
Series Description	(0008,103E)	O	O	-	Single Value, Wildcard, universal
Operator's Name	(0008,1070)	O	O	-	Single Value, Wildcard, universal
Performing Physician's name	(0008,1050)	O	O	-	Single Value, Wildcard, universal
Performed Procedure Step Start Date	(0040,0244)	O	O	-	universal
Performed Procedure Step Start Time	(0040,0245)	O	O	-	universal
Number of Series related Instances	(0020,1209)	O	O	-	universal

Attribute Name	Tag	PR	SR	PSo	Matching
Image or SR Document Level					
SOP Instance UID	(0008,0018)	U	U	-	Single Value, List of UIDs
Image Number	(0020,0013)	R	R	-	Single Value, universal
Content Date	(0008,0023)	O	O	-	Single Value, Range, universal
Content Time	(0008,0033)	O	O	-	Single Value, Range, universal
Modality	(0008,0060)	O	O	-	Single Value, Wildcard, universal
Image Comments	(0020,4000)	O	O	-	universal
Referenced Request Sequence	(0040,A370)	O	O	-	Sequence matching
>Accession Number	((0008,0050)	O	O	-	Single value, universal
>Requested Procedure ID	(0040,1000)	O	O	-	Single value, universal
Concept Name Code Sequence	(0040,A043)	O	O	-	Sequence matching
>Code Value	(0008,0100)	O	O	-	Single Value, Wildcard, universal
>Coding Scheme Designator	(0008,0102)	O	O	-	Single Value, Wildcard, universal
>Coding Scheme Version	(0008,0103)	O	O	-	Single Value, Wildcard, universal
>Code Meaning	(0008,0104)	O	O	-	Single Value, Wildcard, universal
Template Identifier	(0040,DB00)	O	O	-	Single Value, Wildcard, universal
Completion Flag	(0040,A491)	O	O	-	Single Value, Wildcard, universal
Verification Flag	(0040,A493)	O	O	-	Single Value, Wildcard, universal
Verifying Observer Sequence	(0040,A073)	O	O	-	Sequence matching
>Verifying Organization	(0040,A027)	O	O	-	Single Value, Wildcard, universal
>Verifying Date Time	(0040,A030)	O	O	-	Single Value, Range, universal
>Verifying Observer Name	(0040,A075)	O	O	-	Single Value, Wildcard, universal
>Verifying Observer Identification Code Sequence	(0040,A088)	O	O	-	Sequence matching
>>Code Value	(0008,0100)	O	O	-	Single Value, Wildcard, universal
>>Coding Scheme Designator	(0008,0102)	O	O	-	Single Value, Wildcard, universal
>>Coding Scheme Version	(0008,0103)	O	O	-	Single Value, Wildcard, universal
>>Code Meaning	(0008,0104)	O	O	-	Single Value, Wildcard, universal

PR = Patient Root Model, **SR** = Study Root Model, **PSo** = Patient/Study Only Model

U = Unique Key, **R** = Required Key, **O** = Optional Key, **-** = not supported or applicable

The "Process Search Requests" activity can return the following status codes:

Table 20 - Status Codes Process Search Request

Service Status	Meaning	Error Codes	Related Fields
Refused	Out of Resources	A700	(0000,0902)
Failed	Identifier does not match SOP Class	A900	(0000,0901) (0000,0902)
	Unable to process	C001	(0000,0901) (0000,0902)
Cancel	Matching terminated due to Cancel request	FE00	None
Success	Matching is complete - No final Identifier is supplied	0000	None
Pending	Matches are continuing - Current Match is supplied and any Optional Keys were supported in the same manner as Required Keys	FF00	Identifier
	Matches are continuing - Warning that one or more Optional Keys were not supported for existence and/or matching for this identifier	FF01	Identifier

4.2.5.4.2 Activity - Process Retrieve Requests

4.2.5.4.2.1 Description and Sequencing of Activity

The associated activity is to respond to retrieve requests initiated from a foreign SCU. Relational retrieve operation is not supported.

Multiple C-GET or C-MOVE requests over the same association are not supported.

4.2.5.4.2.1 Accepted Presentation Contexts

The syngo DICOM application will accept Presentation Contexts as shown in the following table:

Table 21 - Presentation Context Table "Process Retrieve Requests"

Presentation Context Table					
Abstract Syntax		Transfer Syntax		Role	Ext. Neg.
Name	UID	Name List	UID List		
Patient Root Query/Retrieve Model - GET	1.2.840.10008.5.1.4.1.2.1.3	Implicit VR Little Endian	1.2.840.10008.1.2	SCP	None
		Explicit VR Big Endian	1.2.840.10008.1.2.2		
		Explicit VR Little Endian	1.2.840.10008.1.2.1		
Study Root Query/Retrieve Model - GET	1.2.840.10008.5.1.4.1.2.2.3	Implicit VR Little Endian	1.2.840.10008.1.2	SCP	None
		Explicit VR Big Endian	1.2.840.10008.1.2.2		
		Explicit VR Little Endian	1.2.840.10008.1.2.1		
Patient/Study Only Query/Retrieve Model - GET	1.2.840.10008.5.1.4.1.2.3.3	Implicit VR Little Endian	1.2.840.10008.1.2	SCP	None
		Explicit VR Big Endian	1.2.840.10008.1.2.2		
		Explicit VR Little Endian	1.2.840.10008.1.2.1		
Patient Root Query/Retrieve Model - MOVE	1.2.840.10008.5.1.4.1.2.1.2	Implicit VR Little Endian	1.2.840.10008.1.2	SCP	None
		Explicit VR Big Endian	1.2.840.10008.1.2.2		
		Explicit VR Little Endian	1.2.840.10008.1.2.1		
Study Root Query/Retrieve Model - MOVE	1.2.840.10008.5.1.4.1.2.2.2	Implicit VR Little Endian	1.2.840.10008.1.2	SCP	None
		Explicit VR Big Endian	1.2.840.10008.1.2.2		
		Explicit VR Little Endian	1.2.840.10008.1.2.1		
Patient/Study Only Query/Retrieve Model - MOVE	1.2.840.10008.5.1.4.1.2.3.2	Implicit VR Little Endian	1.2.840.10008.1.2	SCP	None
		Explicit VR Big Endian	1.2.840.10008.1.2.2		
		Explicit VR Little Endian	1.2.840.10008.1.2.1		

Note: C-FIND Extended Negotiation will not be supported.

The order of preference for accepting Transfer Syntaxes is: 1. Explicit VR Little Endian, 2. Explicit VR Big Endian, 3. Implicit VR Little Endian.

4.2.5.4.2.2 SOP Specific Conformance

Relational retrieve operation is not supported.

All unique keys have to be supplied according to the selected Query/Retrieve Level. The related tables in the C-FIND SCP section will give information about "U" marked key attributes.

The C-STORE can only be performed to AEs that are configured in the syngo.

The "Process Retrieve Requests" activity can return the following status codes:

Table 22 - Status Codes "Process Retrieve Requests"

Service Status	Meaning	Error Codes	Related Fields
Refused	Out of Resources - Unable to calculate number of matches	A701	(0000,0902)
	Out of Resources - Unable to perform sub operations	A702	(0000,1020) (0000,1021) (0000,1022) (0000,1023)
Failed	Identifier does not match SOP Class	A900	(0000,0901) (0000,0902)
	Unable to process	C001	(0000,0901) (0000,0902)
Cancel	Sub-operations terminated due to Cancel Indication	FE00	(0000,1020) (0000,1021) (0000,1022) (0000,1023)
Warning	Sub-operations Complete - One or more Failures of Warnings	B000	(0000,1020) (0000,1021) (0000,1022) (0000,1023)
Success	Sub-operations Complete - No Failures or Warning	0000	(0000,1020) (0000,1021) (0000,1022) (0000,1023)
Pending	Sub-operations are continuing	FF00	(0000,1020) (0000,1021) (0000,1022) (0000,1023)

4.2.6 Print SCU Specification

4.2.6.1 SOP Classes

For SOP Classes supported, please refer to “Table 1 - Network Services” section “Print Management” in chapter 1 [“Conformance Statement Overview”](#).

4.2.6.2 Association Policies

4.2.6.2.1 General

Whenever a film-sheet is completely set up and printed by command or automated rule, the job is prepared for processing. As soon as the queue is ready to process the job, it is activated and worked according to the processing data. The Print application will initiate an association to the print destination and process the printing.

The default PDU [size from](#) syngo will be 515KB.

4.2.6.2.2 Number of Associations

The syngo DICOM application initiates one association at a time for each different print device configured.

4.2.6.2.3 Asynchronous Nature

The syngo DICOM print application does not support asynchronous communication (multiple outstanding transactions over a single association).

4.2.6.2.4 Implementation Identifying Information

For Implementation Identifying Information please refer to “Table 3 - Implementation Identifying Information” in chapter 1 [“Conformance Statement Overview”](#).

4.2.6.3 Association Initiation Policy

Triggered by the Print job queue the Print Management SCU establishes an association by using the DICOM association services. An N-GET request determines the printer status prior to printing. If the printer status is “normal”, the print job is started.

After the last film is printed from queue, the Print application will leave open the association for another 60 seconds. If a new film job is ready for printing within this time-limit, the job will be immediately processed over the still open association. If there is no new job, the association is closed.

During the “idle-time” (no open association to printer) the Print application will issue a cyclic camera status request (using N-GET of the Printer SOP Class) every 5 minutes.

4.2.6.3.1 Activity - Print Film

4.2.6.3.1.1 Description and Sequencing of Activity

The film sheet is internally processed, converted to a Standard/1-1 page and then the page image is sent. Status is controlled by awaiting any N-EVENT message through the transfer until the last image or film-sheet is sent.

If the response from the remote application contains a status other than Success or Warning the association is aborted.

4.2.6.3.1.2 Proposed Presentation Context

The syngo DICOM application will propose Presentation Contexts as shown in the following table:

Table 23 - Presentation Context Table "Print Film"

Presentation Context Table					
Abstract Syntax		Transfer Syntax		Role	Ext. Neg.
Name	UID	Name List	UID List		
Basic Grayscale Print Management Meta SOP Class	1.2.840.10008.5.1.1.9	Implicit VR Little Endian Explicit VR Little Endian Explicit VR Big Endian	1.2.840.10008.1.2 1.2.840.10008.1.2.1 1.2.840.10008.1.2.2	SCU	None
Basic Film Session SOP Class	1.2.840.10008.5.1.1.1	Implicit VR Little Endian Explicit VR Little Endian Explicit VR Big Endian	1.2.840.10008.1.2 1.2.840.10008.1.2.1 1.2.840.10008.1.2.2	SCU	None
Basic Film Box SOP Class	1.2.840.10008.5.1.1.2	Implicit VR Little Endian Explicit VR Little Endian Explicit VR Big Endian	1.2.840.10008.1.2 1.2.840.10008.1.2.1 1.2.840.10008.1.2.2	SCU	None
Basic Grayscale Image Box SOP Class	1.2.840.10008.5.1.1.4	Implicit VR Little Endian Explicit VR Little Endian Explicit VR Big Endian	1.2.840.10008.1.2 1.2.840.10008.1.2.1 1.2.840.10008.1.2.2	SCU	None
Printer SOP Class	1.2.840.10008.5.1.1.16	Implicit VR Little Endian Explicit VR Little Endian Explicit VR Big Endian	1.2.840.10008.1.2 1.2.840.10008.1.2.1 1.2.840.10008.1.2.2	SCU	None
Print Job SOP Class	1.2.840.10008.5.1.1.14	Implicit VR Little Endian Explicit VR Little Endian Explicit VR Big Endian	1.2.840.10008.1.2 1.2.840.10008.1.2.1 1.2.840.10008.1.2.2	SCU	None
Presentation LUT SOP Class	1.2.840.10008.5.1.1.23	Implicit VR Little Endian Explicit VR Little Endian Explicit VR Big Endian	1.2.840.10008.1.2 1.2.840.10008.1.2.1 1.2.840.10008.1.2.2	SCU	None

4.2.6.3.1.3 SOP Specific Conformance

The syngo DICOM print management SCU conforms to the DICOM Basic Grayscale Print Management Meta SOP Class.

The application uses a setting platform to define the properties of the connected DICOM SCP, e.g.:

- maximum number of print jobs in the queue
- maximum number of print copies
- supported film sizes of the connected DICOM SCP
- supported film formats of the DICOM SCP
- lookup table definition.

The printing is only suspended in the case of a failure return status of the SCP.

Basic Film Session SOP Class

The Basic Film Session information object definition describes all the user-defined parameters, which are common for all the films of a film session. The Basic Film Session refers to one or more Basic Film Boxes that are printed on one hardcopy printer.

The syngo DICOM print management SCU supports the following DIMSE Service elements for the Basic Film Session SOP Class as SCU:

- N-CREATE
- N-DELETE

The Basic Film Session SOP Class N-CREATE-RQ (SCU) uses the following attributes:

Table 24 - Basic Film Session N-CREATE attributes

Attribute Name	Tag	Usage SCU	Supported Values
Number of Copies	(2000,0010)	U	"1"
Medium Type	(2000,0030)	U	BLUE FILM CLEAR FILM PAPER
Film Destination	(2000,0040)	U	MAGAZINE PROCESSOR

U = User Option

The number of copies sent to the DICOM Printer is always 1, the job is sent n times for n copies.

The affected SOP Instance UID received with N-CREATE-RSP message will be kept internally and used for later requests (e.g. N-DELETE-RQ) on the Basic Film Session – see below:

Attribute Name	Tag	Source of Information
Requested SOP Instance UID	(0000,1000) →(0000,1001)	Affected SOP Instance UID of N-CREATE-RSP on Basic Film Session

The N-DELETE-RQ on the Basic Film Session SOP Class is used to remove the complete Basic Film Session SOP Instance hierarchy.

The Basic Film Session SOP Class interprets the following status codes (from N-CREATE-RSP, N-DELETE-RSP messages):

Table 25 - Basic Film Session Status Codes

Service Status	Meaning	Error Codes
Failure	Film session SOP instances hierarchy does not contain film box SOP instances	C600
	Unable to create print job, print queue is full	C601
	Image size is larger than images box size	C603
Warning	Memory allocation not supported	B600
	Film session printing is not supported	B601
	Film box does not contain image box (empty page)	B602
Success	Film belonging to the film session are accepted for printing	0000

Basic Film Box SOP Class

The Basic Film Box information object definition describes all the user-defined parameter of one film of the film session. The Basic Film Box information description defines the presentation parameters, which are common for all images on a given sheet of film.

The Basic Film Box refers to one or more Image Boxes.

Supported Service Elements as SCU are:

- N-CREATE
- N-ACTION
- N-DELETE

The Basic Film Box SOP Class N-CREATE-RQ message uses the following attributes (the actual values for each attribute depend on DICOM printer configuration within the syngo DICOM print management SCU):

Table 26 - Basic Film Box N-CREATE attributes

Attribute Name	Tag	Usage SCU	Supported Values
Image Display Format	(2010,0010)	M	STANDARD\1,1
Referenced Film Session Sequence	(2010,0500)	M	n. a.
> Referenced SOP Class UID	(0008,1150)	M	1.2.840.10008.5.1.1.1
> Referenced SOP Instance UID	(0008,1155)	M	
Film Orientation	(2010,0040)	M	PORTRAIT
Film Size ID	(2010,0050)	M	8INX10IN, 10INX12IN, 10INX14IN, 11INX14IN,, 14INX14IN, 14INX17IN, 24CMX24CM, 24CMX30CM
Magnification Type	(2010,0060)	M	BILINEAR, CUBIC, NONE, REPLICATE
Max Density	(2010,0130)	U	> 0
Min Density	(2010,0120)	U	50 > value > 0
Illumination	(2010,015E)	U	> 0 Required if Presentation LUT is present.
Reflective Ambient Light	(2010,0160)	U	> 0 Required if Presentation LUT is present.
Referenced Presentation LUT Sequence	(2050,0500)	U	

M = Mandatory, **U** = User Option

The N-CREATE-RSP message from the Print SCP includes the Referenced Image Box Sequence with SOP Class/Instance UID pairs which will be kept internally and used for the subsequent Basic Image Box SOP Class N-SET-RQ messages.

When all Image Boxes (including parameters) for the film-sheet have been set, the DICOM print manager will issue a N-ACTION-RQ message with the SOP Instance UID of the Basic Film Box and the Action Type ID of 1.

The affected SOP Instance UID received with N-CREATE-RSP message will be kept internally and used for later requests (e.g. N-DELETE-RQ) on the Basic Film Box - see below:

Attribute Name	Tag	Source of Information
Requested SOP Instance UID	(0000,1000) →(0000,1001)	Affected SOP Instance UID of N-CREATE-RSP on Basic Film Box

The Basic Film Box SOP Class interprets the following status codes:

Table 27 - Basic Film Box Status Codes

Service Status	Meaning	Error Codes
Failure	Unable to create print job, print queue is full	C601
	Image size is larger than images box size	C603

Service Status	Meaning	Error Codes
Warning	Film box does not contain image box (empty page)	B603
	Requested MinDensity or MaxDensity outside of Printer's operating range	B605
Success	Film accepted for printing	0000

Basic Grayscale Image Box SOP Class

The Basic Grayscale Image Box information object definition is the presentation of an image and image related data in the image area of a film. The Basic Grayscale Image Box information describes the presentation parameters and image pixel data, which apply to a single image of a sheet of film.

The Grayscale Image Box SOP Class uses only the N-SET-RQ with the following attributes:

Table 28 - Basic Grayscale Image Box N-SET attributes

Attribute Name	Tag	Usage SCU	Supported Values
Image Position	(2020,0010)	M	1
BASIC Grayscale Image Sequence	(2020,0110)	M	n.a.
> Samples per Pixel	(0028,0002)	M	1
> Photometric Interpretation	(0028,0004)	M	MONOCHROME2
> Rows	(0028,0010)	M	<Printer/Film config>
> Columns	(0028,0011)	M	<Printer/Film config>
> Pixel Aspect Ratio	(0028,0034)	M	(1:1)
> Bits Allocated	(0028,0100)	M	8, 16
> Bits Stored	(0028,0101)	M	8, 12
> High Bit	(0028,0102)	M	7, 11
> Pixel Representation	(0028,0103)	M	0
> Pixel Data	(7FE0,0010)	M	

M = Mandatory

The Grayscale Image Box SOP Class interprets the following status codes:

Table 29 - Basic Grayscale Image Box Status Codes

Service Status	Meaning	Error Codes
Failure	Image contains more pixel than printer can print in Image Box	C603
	Insufficient memory in printer to store the image	C605
Warning	Requested MinDensity or MaxDensity outside of Printer's operating range	B605
Success		0000

Presentation LUT SOP Class

The Presentation LUT tailors image hardcopy printing for specific modalities, applications and user preferences.

The output of the Presentation LUT is Presentation Values (P-Values). P-Values are approximately related to human perceptual response. They are intended to facilitate common input for hardcopy. P-Values are intended to be independent of the specific class or characteristics of the hardcopy device.

The Presentation LUT SOP Class uses only the N-CREATE-RQ with the following attributes:

Table 30 - Presentation LUT N-CREATE attribute

Attribute Name	Tag	Usage SCU	Supported Values
Presentation LUT Shape	(2050,0020)	U	IDENTITY

U = User Option

The affected SOP Instance UID received with N-CREATE-RSP message will be kept internally and is used for later requests on the Basic Film Box (N-CREATE-RQ) and on the Presentation LUT (N-DELETE-RQ) - see below:

Attribute Name	Tag	Source of Information
Requested SOP Instance UID	(0000,1000) →(0000,1001)	Affected SOP Instance UID of N-CREATE-RSP on Presentation LUT

The Presentation LUT SOP Class interprets the following status codes:

Table 31 - Presentation LUT Status Codes

Service Status	Meaning	Codes
Success	Presentation LUT successfully created	0000
Warning	Requested MinDensity or MaxDensity outside of printer's operating range. The printer will use its respective minimum or maximum density value instead.	B605

Printer SOP Class

The Printer SOP Class allows to monitor the status of the hardcopy printer in a synchronous and an asynchronous way.

The SCU uses the mandatory N-EVENT Report DIMSE service to monitor the changes of the printer status in an asynchronous way.

The following returned information is supported:

Table 32 - Used Printer N-EVENT Report attributes

Event-type Name	Event	Attributes	Tag	Usage SCU
Normal	1			
Warning	2	Printer Status Info	(2110,0020)	U
Failure	3	Printer Status Info	(2110,0020)	U

U = User Option

Table 33 - Mandatory Printer N-GET-RSP, N-EVENT-REPORT-RQ attributes

Attribute Name	Tag	Usage SCP	Supported Values
Printer Status	(2110,0010)	M	NORMAL, FAILURE, WARNING
Printer Status Info	(2110,0020)	M	See tables in Annex for details.

M = Mandatory

Note: For a detailed description on how syngo reacts on different printer status messages, please refer to the Annex section.

Printer Job SOP Class

The Print Job SOP Class allows to monitor the execution of the print process.

The syngo DICOM Print Management application supports the optional N-EVENT-REPORT DIMSE Service to receive the changes of the Print Job Status in an asynchronous way.

It can receive Events from the Print SCP asynchronously:

- N-EVENT-REPORT

Note: The underlying syngo DICOM Print AE does not support receiving of N-EVENT-REPORT messages from camera during open print sessions. This is typically configurable in the camera setup.

The following information is supported:

Table 34 - Used Print Job N-EVENT Report attributes

Event-type Name	Event	Attributes	Tag	Usage SCU
Normal	1	Execution Status Info	(2100,0030)	U
		Print Job ID	(2100,0010)	-- (Print Queue Management SOP Class not supported)
		Film Session Label	(2000,0050)	U
		Printer Name	(2110,0030)	U
Printing	2	Execution Status Info	(2100,0030)	U
		Print Job ID	(2100,0010)	-- (Print Queue Management SOP Class not supported)
		Film Session Label	(2000,0050)	U
		Printer Name	(2110,0030)	U
Done	3	Execution Status Info	(2100,0030)	U
		Print Job ID	(2100,0010)	-- (Print Queue Management SOP Class not supported)
		Film Session Label	(2000,0050)	U
		Printer Name	(2110,0030)	U
Failure	4	Execution Status Info	(2100,0030)	U
		Print Job ID	(2100,0010)	-- (Print Queue Management SOP Class not supported)
		Film Session Label	(2000,0050)	U
		Printer Name	(2110,0030)	U

U = User Option

Note: For a detailed description on how syngo reacts on different printer status messages, please refer to the Annex section.

4.2.6.3.2 Activity - Show Device Status

4.2.6.3.2.1 Description and Sequencing of Activity

With no printing activity ongoing ("idle time"), the syngo DICOM Print SCU application will cyclically request the printer status to update the related printer state in the Printing UI.

4.2.6.3.2.2 Proposed Presentation Context

The syngo DICOM application will propose Presentation Contexts as shown in the following table:

Table 35 - Presentation Context Table "Show Device Status"

Presentation Context Table					
Abstract Syntax		Transfer Syntax		Role	Ext. Neg.
Name	UID	Name List	UID List		
Printer SOP Class	1.2.840.10008.5.1.1.16	Implicit VR Little Endian Explicit VR Little Endian Explicit VR Big Endian	1.2.840.10008.1.2 1.2.840.10008.1.2.1 1.2.840.10008.1.2.2	SCU	None

4.2.6.3.2.3 SOP Specific Conformance

The Printer SOP Class allows to monitor the status of the hardcopy printer in a synchronous and an asynchronous way.

The Print SCU AE application will cyclically “ask” the Printer (SCP) for its status synchronously:

- N-GET as SCU

The following information is supported:

Table 36 - Used Printer N-EVENT Report attributes

Event-type Name	Event	Attributes	Tag	Usage SCU
Normal	1			
Warning	2	Printer Status Info	(2110,0020)	U
Failure	3	Printer Status Info	(2110,0020)	U

U = User Option

4.2.6.4 Association Acceptance Policy

n. a.

4.2.7 Worklist SCU AE

4.2.7.1 SOP Classes

For SOP Classes supported, please refer to “Table 1 - Network Services” section „Workflow Management“ in chapter 1 [“Conformance Statement Overview”](#).

4.2.7.2 Association Policies

4.2.7.2.1 General

It is possible to configure a cyclic update of the modality Scheduler DB through a background worklist request with date/time and modality information.

In addition, the user can request worklist update with “Update Worklist”. No duplicate entries will be added in the Scheduler DB. Entries are uniquely identified by the Study Instance UID (0020,000D) for the Requested Procedure and the SPS ID (0040,009) in the SPS Sequence (0040,0100).

An interactive worklist query can be issued with search criteria entered in the patient based Query dialog from the patient browser..

The default PDU size from syngo will be 515KB.

4.2.7.2.2 Number of Associations

The syngo DICOM application initiates one association at a time to query worklist entry data.

4.2.7.2.3 Asynchronous Nature

The syngo DICOM software does not support asynchronous communication (multiple outstanding transactions over a single association).

4.2.7.2.4 Implementation Identifying Information

For Implementation Identifying Information please refer to “Table 3 - Implementation Identifying Information” in chapter 1 [“Conformance Statement Overview”](#).

4.2.7.3 Association Initiation Policy

The syngo DICOM application will cyclically query the worklist provider and by request from the patient registration interface. It establishes an association by using the

- C-FIND with Worklist information model

It is possible to configure multiple worklist providers but only one can be active at a time. The active worklist provider can be selected in the user settings.

4.2.7.3.1 Activity - (cyclic) Update Worklist

4.2.7.3.1.1 Description and Sequencing of Activity

A network application will perform worklist queries with the C-FIND request at regular intervals. In addition it can be triggered by immediate request. The received worklist items will be compared with the contents of the local Scheduler DB. New items will be inserted into Scheduler DB.

After each broad-query, all Requested Procedures / Scheduled Procedure Steps that were canceled or rescheduled to another modality at the RIS will be automatically removed from the Scheduler DB if :

1. the Examination of this procedure has not been started or finished yet, and

- the corresponding configuration item “Automatic removal of canceled/rescheduled Request” was checked in the Service UI under DICOM/HIS-RIS Node.

No automatic clean-up of the Scheduler DB is performed after a Patient-based Query since the worklist received - due to restricted search criteria - does not correspond to the list of all currently scheduled procedures for the modality.

4.2.7.3.1.2 Proposed Presentation Context

The syngo DICOM application will propose Presentation Contexts as shown in the following table:

Table 37 - Presentation Context “Update Worklist”

Presentation Context Table – “Update Flag Information”				
Abstract Syntax	Transfer Syntax		Role	Ext. Neg.
Description	Name List	UID List		
1.2.840.10008.5.1.4.31 Modality Worklist Information Model – FIND	Explicit VR Little Endian Explicit VR Big Endian Implicit VR Little Endian	1.2.840.10008.1.2.1 1.2.840.10008.1.2.2 1.2.840.10008.1.2	SCU	None

4.2.7.3.1.3 SOP Specific Conformance

Search Key Attributes for the Worklist C-FIND

The syngo DICOM worklist SCU supports “broad worklist queries” with all required search keys. The following table describes the “broad query” search keys that the SCU supports.

Table 38 - Supported Broad Worklist Query Search Key Attributes

Attribute Name	Tag	Matching Key Type	Query Value
Scheduled Procedure Step			
Scheduled Procedure Step Sequence	(0040,0100)	R	
>Scheduled Station AE Title <i>(It depends on user configuration (Options->Configuration-> Patient Registration) if the "own AET" is provided or not. Use the "HIS/RIS" tab card for configuration.)</i>	(0040,0001)	R	<own AET> or <zero length>
>Schedule Procedure Step Start Date <i>(It depends on user configuration (Options->Configuration-> Patient Registration) if the actual Date with a full time range or an interactive input dialog for date/time specification is used.)</i>	(0040,0002)	R	<act. Date>-<act. Date> or range from UI
>Schedule Procedure Step Start Time <i>(It depends on user configuration (Options->Configuration-> Patient Registration) if the actual Date with a full time range or an interactive input dialog for date/time specification is used.)</i>	(0040,0003)	R	00.00-235959.00 or range from UI
>Modality <i>(It depends on user configuration (Options->Configuration-> Patient Registration) if the "own Modality" is provided or not. Use the "HIS/RIS" tab card for configuration.)</i>	(0008,0060)	R	<zero length> or <own Modality>

R = Required

Return Key Attributes of the Worklist C-FIND

The syngo DICOM Worklist SCU supports worklist queries with return key attributes of all types. The following table describes the return keys that the SCU supports.

An “x” in the **UI** column will indicate the attribute is displayed in the user interface. The display is influenced by the related configuration.

A tag in the **IOD** column will indicate that the related attribute is included into the SOP Instances of the IODs created during processing of this worklist request.

A tag in the **MPPS** column will indicate that the related attribute is included into the SOP Instances of the MPPS objects created during processing of this worklist request. (See also the tables “Attributes used for the Performed Procedure Step N-CREATE” and “Attributes used for the Performed Procedure Step N-SET”.)

Table 39 - Basic Worklist C-FIND-RSP Return Key Attributes

Attribute Name	Tag	Return Key Type	UI	IOD	MPPS
SOP Common					
Specific Character Set	(0008,0005)	1C	-	(0008,0005)	(0008,0005)
Scheduled Procedure Step					
Scheduled Procedure Step Sequence	(0040,0100)	1			
>Modality	(0008,0060)	1	x	(0008,0060)	(0008,0060)
>Requested Contrast Agent	(0032,1070)	2C	x		
>Scheduled Station AE Title (“Scheduled Station AE Title” is taken as default for “Performed Station AE Title”)	(0040,0001)	1	x		(0040,0241)
>Scheduled Procedure Step Start Date	(0040,0002)	1	x		
>Scheduled Procedure Step Start Time	(0040,0003)	1	x		
>Scheduled Procedure Step End Date	(0040,0004)	3	-		
>Scheduled Procedure Step End Time	(0040,0005)	3	-		
>Scheduled Performing Physician’s Name (“Scheduled Performing Physician’s Name” is taken as default for “Performing Physician’s Name”)	(0040,0006)	1	x	(0008,1050)	(0008,1050)
>Scheduled Procedure Step Description (“Scheduled Procedure Step Description” is taken as default for “Performed Procedure Step Description”)	(0040,0007)	1C	x	(0040,0007) (0040,0254)	(0040,0007) (0040,0254)
>Scheduled Protocol Code Sequence (universal Sequence Match) (“Scheduled Protocol Code Sequence” is taken as default for “Performed Protocol Code Sequence”)	(0040,0008)	1C	-	(0040,0008) (0040,0260)	(0040,0008) (0040,0260)
>>Code Value	(0008,0100)	1C	x		
>>Coding Scheme Designator	(0008,0102)	1C	x		
>>Coding Scheme Version	(0008,0103)	3	x		
>>Code Meaning	(0008,0104)	3	x		
>Scheduled Procedure Step ID (“Scheduled Procedure Step ID” is taken as default for “Performed Procedure Step ID”)	(0040,0009)	1	x	(0040,0009) (0040,0253)	(0040,0009) (0040,0253)
>Scheduled Station Name	(0040,0010)	2	x		
>Scheduled Procedure Step Location (“Scheduled Procedure Step Location” is taken as default for “Performed Location”)	(0040,0011)	2	x		(0040,0243)
>Pre-Medication	(0040,0012)	2C	x		
>Scheduled Procedure Step Status	(0040,0020)	3	x		
>Comments on the Scheduled Procedure Step	(0040,0400)	3	-		
Requested Procedure					
Referenced Study Sequence (universal)	(0008,1110)	2	-	(0008,1110)	(0008,1110)

Attribute Name	Tag	Return Key Type	UI	IOD	MPPS
<i>Sequence Match</i>					
>Referenced SOP Class UID	(0008,1150)	1C	-		
>Referenced SOP Instance UID	(0008,1155)	1C	-		
Study Instance UID	(0020,000D)	1	-	(0020,000D)	(0020,000D)
Requested Procedure Description	(0032,1060)	1C	x	(0032,1060)	(0032,1060)
Requested Procedure Code Sequence (<i>universal Sequence Match</i>) (<i>“Requested Procedure Code Sequence” is taken as default for “Procedure Code Sequence”</i>)	(0032,1064)	1C	-	(0008,1032) (0032,1064)	(0008,1032)
>Code Value	(0008,0100)	1C	x		
>Coding Scheme Designator	(0008,0102)	1C	x		
>Coding Scheme Version	(0008,0103)	3	x		
>Code Meaning	(0008,0104)	3	x		
Requested Procedure ID (<i>“Requested Procedure ID” is taken as default for “Study ID”</i>)	(0040,1001)	1	x	(0040,1001) (0020,0010)	(0040,1001) (0020,0010)
Reason for the Requested Procedure	(0040,1002)	3	-	(0040,1002)	
Requested Procedure Priority	(0040,1003)	2	x		
Patient Transport Arrangements	(0040,1004)	2	-		
Requested Procedure Location	(0040,1005)	3	-		
Confidentiality Code	(0040,1008)	3	-		
Reporting Priority	(0040,1009)	3	-		
Names of intended Recipients of Results	(0040,1010)	3	-	(0008,1048)	
Requested Procedure Comments	(0040,1400)	3	x		
Imaging Service Request					
Accession Number	(0008,0050)	2	x	(0008,0050)	(0008,0050)
Referring Physician's Name	(0008,0090)	2	x	(0008,0090)	
Requesting Physician	(0032,1032)	2	x	(0032,1032) (0008,1048)	
Requesting Service	(0032,1033)	3	x	(0032,1033)	
Issuing Date of Imaging Service Request	(0040,2004)	3	-		
Issuing Time of Imaging Service Request	(0040,2005)	3	-		
Placer Order Number / Imaging Service Request (<i>Old tag (0040,2006) is retired and not used.</i>)	(0040,2016)	3	-		(0040,2016)
Filler Order Number / Imaging Service Request (<i>Old tag (0040,2007) is retired and not used.</i>)	(0040,2017)	3	-		(0040,2017)
Order entered by ...	(0040,2008)	3	-		
Order Enterer's location	(0040,2009)	3	-		
Order Callback Phone Number	(0040,2010)	3	-		
Imaging Service Request Comments	(0040,2400)	3	x		
Visit Identification					
Institution Name	(0008,0080)	3	x	(0008,0080)	
Institution Address	(0008,0081)	3	-		
Institution Code Sequence (<i>universal Sequence Match</i>)	(0008,0082)	3	-		

Attribute Name	Tag	Return Key Type	UI	IOD	MPPS
>Code Value	(0008,0100)	1C	-		
>Coding Scheme Designator	(0008,0102)	1C	-		
>Coding Scheme Version	(0008,0103)	3	-		
>Code Meaning	(0008,0104)	3	-		
Admission ID	(0038,0010)	2	x		
Issuer of Admission ID	(0038,0011)	3	-		
Visit Status					
Visit Status ID	(0038,0008)	3	-		
Current Patient Location	(0038,0300)	2	x		
Patient's Institution Residence	(0038,0400)	3	-		
Visit Comments	(0038,4000)	3	-		
Visit Relationship					
Referenced Study Sequence (<i>universal Sequence Match</i>)	(0008,1110)	3	-		
>Referenced SOP Class UID	(0008,1150)	1C	-		
>Referenced SOP Instance UID	(0008,1155)	1C	-		
Referenced Patient Sequence (<i>universal Sequence Match</i>)	(0008,1120)	2	-		(0008,1120)
>Referenced SOP Class UID	(0008,1150)	1C	-		
>Referenced SOP Instance UID	(0008,1155)	1C	-		
Visit Admission					
Referring Physician's Name	(0008,0090)	2	x	(0008,0090)	
Admitting Diagnosis Description	(0008,1080)	3	x	(0008,1080)	
Patient Identification					
Patient's Name	(0010,0010)	1	x	(0010,0010)	(0010,0010)
Patient ID	(0010,0020)	1	x	(0010,0020)	(0010,0020)
Issuer of Patient ID	(0010,0021)	3	-	(0010,0021)	
Other Patient IDs	(0010,1000)	3	x	(0010,1000)	
Other Patient Names	(0010,1001)	3	x	(0010,1001)	
Patient's Birth Name	(0010,1005)	3	-	(0010,1005)	
Patient's Mother's Birth Name	(0010,1060)	3	-	(0010,1060)	
Medical Record Locator	(0010,1090)	3	-	(0010,1090)	
Patient Demographic					
Patient's Birth Date	(0010,0030)	2	x	(0010,0030)	(0010,0030)
Patient's Birth Time	(0010,0032)	3	-	(0010,0032)	
Patient's Sex	(0010,0040)	2	x	(0010,0040)	(0010,0040)
Patient's Insurance Plan Code Sequence (<i>universal Sequence Match</i>)	(0010,0050)	3	-	(0010,0050)	
>Code Value	(0008,0100)	1C	-		
>Coding Scheme Designator	(0008,0102)	1C	-		
>Coding Scheme Version	(0008,0103)	3	-		
>Code Meaning	(0008,0104)	3	-		
Patient's Age	(0010,1010)	3	x	(0010,1010)	
Patient's Size	(0010,1020)	3	x	(0010,1020)	
Patient's Weight	(0010,1030)	2	x	(0010,1030)	
Patient's Address	(0010,1040)	3	x	(0010,1040)	
Military Rank	(0010,1080)	3	x	(0010,1080)	
Branch of Service	(0010,1081)	3	-	(0010,1081)	
Country of Residence	(0010,2150)	3	-	(0010,2150)	
Region of Residence	(0010,2152)	3	-	(0010,2152)	
Patient's Telephone Numbers	(0010,2154)	3	-	(0010,2154)	

Attribute Name	Tag	Return Key Type	UI	IOD	MPPS
Ethnic Group	(0010,2160)	3	x	(0010,2160)	
Occupation	(0010,2180)	3	-	(0010,2180)	
Patient's Religious Preference	(0010,21F0)	3	-	(0010,21F0)	
Patient Comments	(0010,4000)	3	x	(0010,4000)	
Patient Data Confidentiality Constraint Description	(0040,3001)	2	x	(0040,3001)	
Patient Medical					
Medical Alerts	(0010,2000)	2	x	(0010,2000)	
Contrast Allergies	(0010,2110)	2	x	(0010,2110)	
Pregnancy Status	(0010,21C0)	2	x	(0010,21C0)	
Smoking Status	(0010,21A0)	3	x	(0010,21A0)	
Last Menstrual Date	(0010,21D0)	3	x	(0010,21D0)	
Additional Patient History	(0010,21B0)	3	x	(0010,21B0)	
Special Needs	(0038,0050)	2	x	(0038,0050)	
Patient State	(0038,0500)	2	x	(0038,0500)	
Patient Relationship					
Referenced Study Sequence (<i>universal Sequence Match</i>)	(0008,1110)	3	-		
>Referenced SOP Class UID	(0008,1150)	1C	-		
>Referenced SOP Instance UID	(0008,1155)	1C	-		
Referenced Visit Sequence (<i>universal Sequence Match</i>)	(0008,1125)	3	-		
>Referenced SOP Class UID	(0008,1150)	1C	-		
>Referenced SOP Instance UID	(0008,1155)	1C	-		
Referenced Patient Alias Sequence (<i>universal Sequence Match</i>)	(0038,0004)	3	-		
>Referenced SOP Class UID	(0008,1150)	1C	-		
>Referenced SOP Instance UID	(0008,1155)	1C	-		

The Worklist SCU interprets the following status codes:

Table 40 - Status Codes "Update Worklist"

Service Status	Meaning	Error Codes	Related Fields
Refused	Out of Resources	A700	(0000,0902)
Failed	Identifier does not match SOP Class	A900	(0000,0901) (0000,0902)
	Unable to process	Cxxx	(0000,0901) (0000,0902)
Cancel	Matching terminated due to Cancel request	FE00	None
Success	Matching is complete - No final Identifier is supplied	0000	None
Pending	Matches are continuing - Current Match is supplied and any Optional Keys were supported in the same manner as Required Keys	FF00	Identifier
	Matches are continuing - Warning that one or more Optional Keys were not supported for existence and/or matching for this identifier	FF01	Identifier

4.2.7.3.2 Activity - Get Worklist

4.2.7.3.2.1 Description and Sequencing of Activity

With "Get Worklist" in the patient based Worklist Query dialog, the entered attributes are used to form a worklist request identifier. The response data is used to fill the Patient Registration dialog. The response data are additionally placed in the Scheduler DB.

4.2.7.3.2.2 Proposed Presentation Context

This Activity will propose the same Presentation Context as with “Update Worklist”. Please see related table in section 4.2.7.3.1.2.

4.2.7.3.2.3 SOP Specific Conformance

The syngo DICOM worklist SCU supports “narrow worklist queries” with all required search keys. The following tables describe the “narrow query” search keys that the SCU supports.

Table 41 - Patient based "narrow query" Search Key Attributes

Attribute Name	Tag	Matching Key Type	Query Value
Scheduled Procedure Step			
Scheduled Procedure Step Sequence	(0040,0100)	R	
>Scheduled Performing Physician’s Name	(0040,0006)	R	Input from UI or <zero length>
Requested Procedure			
Requested Procedure ID	(0040,1001)	O	Input from UI or <zero length>
Imaging Service Request			
Accession Number	(0008,0050)	O	Input from UI or <zero length>
Referring Physician’s Name	(0008,0090)	O	Input from UI or <zero length>
Visit Status			
Current Patient Location	(0038,0300)	O	Input from UI or <zero length>
Patient Identification			
Patient’s Name	(0010,0010)	R	Input from UI or <zero length>
Patient ID	(0010,0020)	R	Input from UI or <zero length>

R = Required Key, **O** = Optional Key

The Return Key Attribute handling and supported Status Codes are identical to the “Update Worklist” activity. Please see 4.2.7.3.1.3 for details.

4.2.7.4 Association Acceptance Policy

n. a.

4.2.8 Modality PPS SCU AE

4.2.8.1 SOP Classes

For SOP Classes supported, please refer to “Table 1 - Network Services” section „Workflow Management“ in chapter 1 [“Conformance Statement Overview”](#).

4.2.8.2 Association Policies

4.2.8.2.1 General

The creation of MPPS Instance is done automatically by syngo whenever a patient is registered for image acquisition through the Patient Registration dialog.

Further updates on the MPPS data can be done interactively from the related MPPS user interface. The MPPS “Complete” or “Discontinued” states can be set from user interface.

The default PDU size from syngo will be 515KB.

4.2.8.2.2 Number of Associations

The syngo DICOM application initiates one association at a time to create or set the MPPS instance.

4.2.8.2.3 Asynchronous Nature

The syngo DICOM software does not support asynchronous communication (multiple outstanding transactions over a single association).

4.2.8.2.4 Implementation Identifying Information

For Implementation Identifying Information please refer to “Table 3 - Implementation Identifying Information” in chapter 1 [“Conformance Statement Overview”](#).

4.2.8.3 Association Initiation Policy

The syngo DICOM application will notify a RIS (MPPS Manager) about the status of a procedure while it is performed. It establishes an association by using the

- N-CREATE DIMSE according to the CREATE Modality Performed Procedure Step SOP Instance operation or a
- N-SET DIMSE to update the contents and state of the MPPS according to the SET Modality Performed Procedure Step Information operation.

It is possible to configure multiple MPPS providers but only one can be active at a time. The active MPPS provider can be selected in the user settings.

4.2.8.3.1 Activity - Patient registered

4.2.8.3.1.1 Description and Sequencing of Activity

A patient is registered by the Patient Registration “Exam” action. From this event the trigger to create a MPPS Instance is derived. The related Instance is then immediately communicated to the configured RIS system. An association is established and the MPPS Instance is sent.

4.2.8.3.1.2 Proposed Presentation Context

The syngo DICOM application will propose Presentation Contexts as shown in the following table:

Table 42 - Presentation Context “Patient Registered”

Presentation Context Table – “Update Flag Information”				
Abstract Syntax	Transfer Syntax		Role	Ext. Neg.
Description	Name List	UID List		
1.2.840.10008.3.1.2.3.3 Modality Performed Procedure Step	Explicit VR Little Endian Explicit VR Big Endian Implicit VR Little Endian	1.2.840.10008.1.2.1 1.2.840.10008.1.2.2 1.2.840.10008.1.2	SCU	None

4.2.8.3.1.3 SOP Specific Conformance

Attributes for the Performed procedure Step N-CREATE

The Siemens syngo DICOM Modality Performed Procedure Step SCU informs the remote SCP when the examination of a scheduled procedure step will be performed (i.e. the patient is registered). The N-CREATE message is sent when the examination is started with successful registration of the patient data. The following table describes the supported attributes of a N-CREATE message.

Table 43 - Performed Procedure Step N-CREATE Attributes

Attribute Name	Tag	Type	Value
SOP Common			
Specific Character Set	(0008,0005)	1C	from MWL or created
Performed Procedure Step Relationship			
Scheduled Step Attribute Sequence	(0040,0270)	1	
>Study Instance UID	(0020,000D)	1	from MWL or created
>Referenced Study Sequence	(0008,1110)	2	from MWL or <zero length>
>>Referenced SOP Class UID	(0008,1150)	1C	
>>Referenced SOP Instance UID	(0008,1155)	1C	
>Accession Number	(0008,0050)	2	from MWL or user input
>Placer Order Number/Imaging Service Request	(0040,2016)	3	from MWL or <zero length>
>Filler Order Number/Imaging Service Request	(0040,2017)	3	from MWL or <zero length>
>Requested Procedure ID	(0040,0001)	2	from MWL or user input
>Requested Procedure Description	(0032,1060)	2	from MWL or <zero length>
>Scheduled Procedure Step ID	(0040,0009)	2	from MWL or <zero length>
>Scheduled Procedure Step Description	(0040,0007)	2	from MWL or <zero length>
>Scheduled Protocol Code Sequence	(0040,0008)	2	from MWL or <zero length>
>>Code Value	(0008,0100)	1C	
>>Coding Scheme Designator	(0008,0102)	1C	
>>Coding Scheme Version	(0008,0103)	3	
>>Code Meaning	(0008,0104)	3	
Patient’s Name	(0010,0010)	2	from MWL or user input
Patient ID	(0010,0020)	2	from MWL or user input
Patient’s Birth Date	(0010,0030)	2	from MWL or user input
Patient’s Sex	(0010,0040)	2	from MWL or user input
Referenced Patient Sequence	(0008,1120)	2	from MWL or <zero length>
>Referenced SOP Class UID	(0008,1150)	1C	
>Referenced SOP Instance UID	(0008,1155)	1C	
Performed Procedure Step Information			
Performed Procedure Step ID	(0040,0253)	1	From SPS ID or created
Performed Station AE Title	(0040,0241)	1	own AE Title
Performed Station Name	(0040,0242)	2	own hostname
Performed Location	(0040,0243)	2	from SPS location or <zero length>
Performed Procedure Step Start Date	(0040,0244)	1	created

Attribute Name	Tag	Type	Value
Performed Procedure Step Start Time	(0040,0245)	1	created
Performed Procedure Step Status	(0040,0252)	1	"IN PROGRESS"
Performed Procedure Step Description	(0040,0254)	2	from SPS Description or <zero length>
Performed Procedure Type Description	(0040,0255)	2	<zero length>
Procedure Code Sequence	(0008,1032)	2	from Requested Procedure Code or <zero length>
>Code Value	(0008,0100)	1C	
>Coding Scheme Designator	(0008,0102)	1C	
>Coding Scheme Version	(0008,0103)	3	
>Code Meaning	(0008,0104)	3	
Performed Procedure Step End Date	(0040,0250)	2	<zero length>
Performed Procedure Step End Time	(0040,0251)	2	<zero length>
Comments on the Performed Procedure Steps	(0040,0280)	3	<zero length>
Image Acquisition Results			
Modality	(0008,0060)	1	XA
Study ID	(0020,0010)	2	from Requested Procedure ID or created
Performed Protocol Code Sequence	(0040,0260)	2	from Scheduled Protocol Code Sequence or <zero length>
>Code Value	(0008,0100)	1C	
>Coding Scheme Designator	(0008,0102)	1C	
>Coding Scheme Version	(0008,0103)	3	
>Code Meaning	(0008,0104)	3	
Performed Series Sequence	(0040,0340)	2	
>Performing Physician's Name	(0008,1050)	2C	from MWL or user input
>Operator's Name	(0008,1070)	2C	User input
>Series Instance UID	(0020,000E)	1C	created
>Series Description	(0008,103E)	2C	<zero length>
>Retrieve AE Title	(0008,0054)	2C	<zero length>
>Protocol Name	(0018,1030)	1C	from organ program
>Referenced Image Sequence	(0008,1140)	2C	<zero length>
>Referenced Non-Image Composite SOP Instance Sequence	(0040,0220)	2C	<zero length>
Radiation Dose			
Anatomic Structure, Space or Region Sequence	(0008,2229)	3	<zero length>
Total Time of Fluoroscopy	(0040,0300)	3	<zero length>
Total Number of Exposures	(0040,0301)	3	<zero length>
Distance Source to Detector	(0018,1110)	3	<zero length>
Distance Source to Entrance	(0040,0306)	3	<zero length>
Entrance Dose	(0040,0302)	3	<zero length>
Entrance Dose in mGy	(0040,8302)	3	<zero length>
Exposed Area	(0040,0303)	3	<zero length>
Image and Fluoroscopy Area Dose Product	(0018,115E)	3	<zero length>
Comments on Radiation Dose	(0040,0310)	3	<zero length>
Exposure Dose Sequence	(0040,030E)	3	<zero length>
Billing and Material Management Code			
Billing Procedure Step Sequence	(0040,0320)	3	<zero length>
Film Consumption Sequence	(0040,0321)	3	
>Number of Films	(2100,0170)	3	<zero length>
>Medium Type	(2000,0030)	3	<zero length>

Attribute Name	Tag	Type	Value
>Film Size ID	(2010,0050)	3	<zero length>
Billing Supplies and Devices Sequence	(0040,0324)	3	
>Billing Item Sequence	(0040,0296)	3	<zero length>
>Quantity Sequence	(0040,0293)	3	
>>Quantity	(0040,0294)	3	<zero length>
>>Measuring Units Sequence	(0040,0295)	3	<zero length>

The Performed Procedure Step SCU interprets the following N-CREATE status codes:

Table 44 - Status Codes "Patient Registered"

Service Status	Meaning	Error Codes (0000.0900)
Failure	Processing Failure	0110
	No such attribute	0105
	Invalid attribute value	0106
	Duplicate SOP Instance	0111
	No such SOP Instance	0112
	No such SOP Class	0118
	Class Instance conflict	0119
	Missing attribute	0120
	Missing attribute value	0121
	Resource limitation	0213
Success	MPPS Instance created	0000

4.2.8.3.2 Activity - MPPS Update

4.2.8.3.2.1 Description and Sequencing of Activity

With the MPPS UI the status of the MPPS Instance can be set to "COMPLETED" or "DISCONTINUED". During performance of the procedure the status will remain "IN PROGRESS".

4.2.8.3.2.2 Proposed Presentation Context

For "MPPS Update" the same Presentation Contexts as with "Patient registered" are proposed. Please see related table in section 4.2.8.3.1.2.

4.2.8.3.2.3 SOP Specific Conformance

Attributes for the Performed procedure Step N-SET

The Siemens syngo DICOM Modality Performed Procedure Step SCU informs the remote SCP about the performed examination and its status. The N-SET message is sent after each acquisition (status "IN PROGRESS") and per finished examination (finished status "COMPLETED" or incomplete status "DISCONTINUED"). The following table describes the supported attributes of a N-SET message.

Table 45 - Performed Procedure Step N-SET Attributes

Attribute Name	Tag	Type	Value
Performed Procedure Step Information			
Performed Procedure Step Status	(0040,0252)	3	"IN PROGRESS" during procedure, "COMPLETED" or "DISCONTINUED" for final N-SET
Performed Procedure Step Description	(0040,0254)	3	from SPS Description or user input
Procedure Code Sequence	(0008,1032)	3	from Requested Procedure
>Code Value	(0008,0100)	1C	
>Coding Scheme Designator	(0008,0102)	1C	
>Coding Scheme Version	(0008,0103)	3	
>Code Meaning	(0008,0104)	3	

Attribute Name	Tag	Type	Value
Performed Procedure Step End Date	(0040,0250)	1	created
Performed Procedure Step End Time	(0040,0251)	1	created
Comments on the Performed Procedure Steps	(0040,0280)	3	user input
Image Acquisition Results			
Performed Protocol Code Sequence	(0040,0260)	3	from Scheduled Protocol Code Sequence
>Code Value	(0008,0100)	1C	
>Coding Scheme Designator	(0008,0102)	1C	
>Coding Scheme Version	(0008,0103)	3	
>Code Meaning	(0008,0104)	3	
Performed Series Sequence	(0040,0340)	1	
>Performing Physician's Name	(0008,1050)	2C	from MWL or user input
>Protocol Name	(0018,1030)	1C	from related SOP Instance
>Operator's Name	(0008,1070)	2C	user input
>Series Instance UID	(0020,000E)	1C	from related SOP Instance
>Series Description	(0008,103E)	2C	from related SOP Instance
>Retrieve AE Title	(0008,0054)	2C	
>Referenced Image Sequence	(0008,1140)	2C	Series related SOP Instances as items
>>Referenced SOP Class UID	(0008,1150)	1C	
>>Referenced SOP Instance UID	(0008,1155)	1C	
>Referenced Standalone SOP Instance Sequence	(0040,0220)	2C	<zero length>
Radiation Dose			
Total Time of Fluoroscopy	(0040,0300)	3	
Total Number of Exposures	(0040,0301)	3	
Entrance Dose in mGy	(0040,8302)	3	accumulated over complete procedure step
Image and Fluoroscopy Area Dose Product	(0018,115E)	3	accumulated over complete procedure step (dGy*cm ²)
Exposure Dose Sequence	(0040,030E)	3	on item for each irradiation event (acquisition or fluoro)
>Radiation Mode	(0018,115A)	3	"PULSED"
>KVP	(0018,0060)	3	peak KV used for this event (KV)
>X-ray Tube Current in µA	(0018,8151)	3	tube current used for this event
>Exposure Time	(0018,1150)	3	time of x-ray in ms for this event
>Comments on Radiation Dose	(0040,0310)	3	additional acquisition specific information (Entrance Dose, Dose Area Product, X-Ray Filter, etc.) as text
Comments on Radiation Dose	(0040,0310)	3	user input
Billing and Material Management Code			
Film Consumption Sequence	(0040,0321)	3	
>Number of Films	(2100,0170)	3	
>Medium Type	(2000,0030)	3	
>Film Size ID	(2010,0050)	3	

The Performed Procedure Step SCU interprets the following N-SET status codes:

Table 46 - Status Codes "MPPS Update"

Service Status	Meaning	Error Codes (0000.0900)
Failure	Processing Failure: Performed Procedure Step Object may no longer be updated.	0110
	No such attribute	0105
	Invalid attribute value	0106
	No such SOP Instance	0112
	Invalid Object instance	0117
	No such SOP Class	0118
	Class Instance conflict	0119
	Missing attribute value	0121
	Resource limitation	0213
Success	MPPS Instance set	0000

Performed Procedure Step ID without MPPS option
 Handling of Performed Procedure Step ID in case

- MPPS is not configured or
- Unscheduled case

The attribute "Performed Procedure Step ID" (0040,0235) will be encoded based on "YYYYMMDDHHMMSS". This date and time is based on the time when the first image is acquired. The "Performed Procedure Step ID" stays the same for all acquired or derived images as long as the patient is re-registered. A re-registered patient with a new study or new series within the existing study will get a newly assigned "Performed Procedure Step ID".

4.2.8.4 Association Acceptance Policy

n. a.

4.3 Network Interfaces

4.3.1 Physical Network Interface

The DICOM Interface of the syngo provides DICOM TCP/IP Network Communication Support and uses the TCP/IP protocol stack from the operating system. It uses the MergeCOM subroutine library. All available Ethernet interfaces are supported.

4.3.2 Additional Protocols

n.a

4.3.3 IPv4 and IPv6 Support

syngo supports the transfer of the DICOM images over the network nodes and workstations using IPv4 and optionally IPv6 protocols using Transfer/Send to features.

Exporting of the images to a network shared folder using Export to offline feature using IPv4 and optionally using IPv6 protocols.

4.4 Configuration

4.4.1 AE Title/Presentation Address Mapping

Local AE Titles

According to the DICOM Standard, the AET string can be up to 16 characters long and must not contain any extended characters, only 7-bit ASCII characters (excluding Control Characters).

Note: The current implementation of *syngo* does not allow Spaces and special characters (like &<> ") in the AE title string.

Change of the default AE Titles chosen by the system can be performed in the Service UI under "Configuration / DICOM / General" item - first page.

Table 47 - Default AET Characteristics

Application Entity	Default AE Title	TCP/IP Port
Verification SCU	RANDOM_STR RANDOM_STR_S	-
Verification SCP		2762(fixed) 104 (fixed)
Storage SCU		-
Storage SCP		2762(fixed) 104 (fixed)
Query/Retrieve SCU		-
Query/Retrieve SCP		2762(fixed) 104 (fixed)
Print SCU	RANDOM_STR	-
Worklist SCU	RANDOM_STR	-
MPPS SCU		-

Port 2762 is used for Secure DICOM Communication and Port 104 is used for Unsecure DICOM Communication. There are two AET for Storage SCP, Verification SCP and Query/Retrieve SCP. RANDOM_STR denotes

the random AET value is randomly generated. RANDOM_STR_S denotes random Aet value for Secure DICOM communication.

Remote AE Titles

When "trusted host functionality" is enabled all external AE Titles have to be configured to be able to communicate with syngo.

For each remote AE the following data and capabilities can be configured:

Table 48 - Remote AE Configuration Items

Remote AE configuration item	Comment
Host Name	As defined in the network domain. This has to be configured also for any DICOM AE that wishes to connect to SCP services of syngo.
TCP/IP address	As defined in the network domain. This has to be configured also for any DICOM AE that wishes to connect to SCP services of syngo.
Logical Name	Name for the AE used in the user interfaces of the syngo applications.
AE Title	AET, as provided by network administration
Port Number	Port Number, as provided by network administration
If Storage Service support is checked	
Transfer Syntax	Selection of uncompressed transfer Syntaxes supported by remote AE
Compression	Selection of additional compression Syntaxes supported for remote AE
Default Node	"first default"/"second default"/["no default"] - activating this feature will show "Send to <logical name>" in the Transfer tool menu for quick access.
Preference Node	When checked, the remote AE will be assigned to a keyboard shortcut key.
Archive Node	When checked, sending to remote AET will set status of a (rchived), else s (ent) is indicated.
Default Archive	When checked, the remote AE will be listed as default archive in User interfaces.
Graphics in Pixel Data	When checked, the DICOM overlay will not be encoded in attribute (60xx,3000) Overlay Data, but masked in the "unused bits" of the pixel data (only for uncompressed transfer syntaxes). For backwards compatibility with legacy AE.
Select SC node	Select a previously configured node as target for Storage Commitment when sending DICOM objects to the configured AE. Default is the same node as to which the Objects are sent.
Select SC AET	Select AET that corresponds to the above selected node that receives the Storage Commitment request. Default is the above specified "AE Title".
SC Result in same association	When checked the syngo DICOM application will await the Storage Commitment N-EVENT-REPORT on the same association. Default is "not checked" (= different association).
SC result timeout	Timeout in hours and minutes to wait at the open association. Default: 01:00 (hour:minutes).
If Storage Commitment Service support is checked	
n. a.	The related Storage Commitment configuration is either in the Storage section of the same AET or different AET (in case the current AET is only Storage Commitment Provider).
If Query Service support is checked	
provides DICOM Query model	The Query models supported by this AET can be selected. When possible, the STUDY ROOT model should preferably be configured
If Retrieve Service support is checked	
n. a.	Checking Retrieve support for an AET is the only needed configuration item. This will allow access to the "Import" feature in the Query result browser.
If Modality Worklist Service support is checked	
Query Waiting time	The time to wait for the C-FIND-RSP after sending the C-FIND-RQ (default

	20 sec.)
Max Query Match Number	The maximum number of entries accepted in one worklist (default is 200)
Query Interval	The time between two C-FIND-RQ to the Hospital Information system (default is 60 min, minimum is 3 min, maximum is 1440 min i.e. 24 hours)
Automatic removal of canceled/rescheduled Requests	Checking this item will removed all unused entries from the scheduler list prior to inserting the worklist responses with each query.

4.4.2 Parameters

System parameters can be changed in the Service UI under “Configuration / DICOM / General” item - second page.

Table 49 - General parameter settings and timeouts

Time-out Values				
Parameter	Default Value[sec]	Min [sec]	Max [sec]	Comment
Accepting/Rejecting an Association Request	60	15	600	Wait for an Association Request or wait for a Peer to shut down the Association
Association Open Request	60	15	600	Wait for a reply to an Association Accept Request
Association Close Request	60	15	600	Wait for a reply to an Association Release Request
Accepting a Message over Network	60	15	600	Wait for a Network Write to be accepted
Waiting for Data between TCP/IP Packets	60	15	600	Wait for Data between TCP/IP packets
Response from Remote Node for Storage/Query/Retrieve	600	15	600	Time between Service Request and Service Response
Accept network connect	60	15	600	
General Transfer Setting				
Simultaneous DICOM associations	10	1	10	Number of simultaneous associations running.
Maximum PDU Size	515kByte	4kByte	1MByte	Proposed PDU size, each selectable value is doubled from previous, starting with 4kB. Additionally for optimization for some networks 28kByte are provided.

5 (DICOM) Media Interchange / Offline Media Interchange

The following "Offline Media Application Profiles (incl. private extensions)" are supported by syngo archive options.

Table 50 - Supported Application Profiles

Application Profile
Basic Cardiac
1024 Extended Cardiac
General Purpose CDR

5.1 Implementation Model

5.1.1 Application Data Flow Diagram

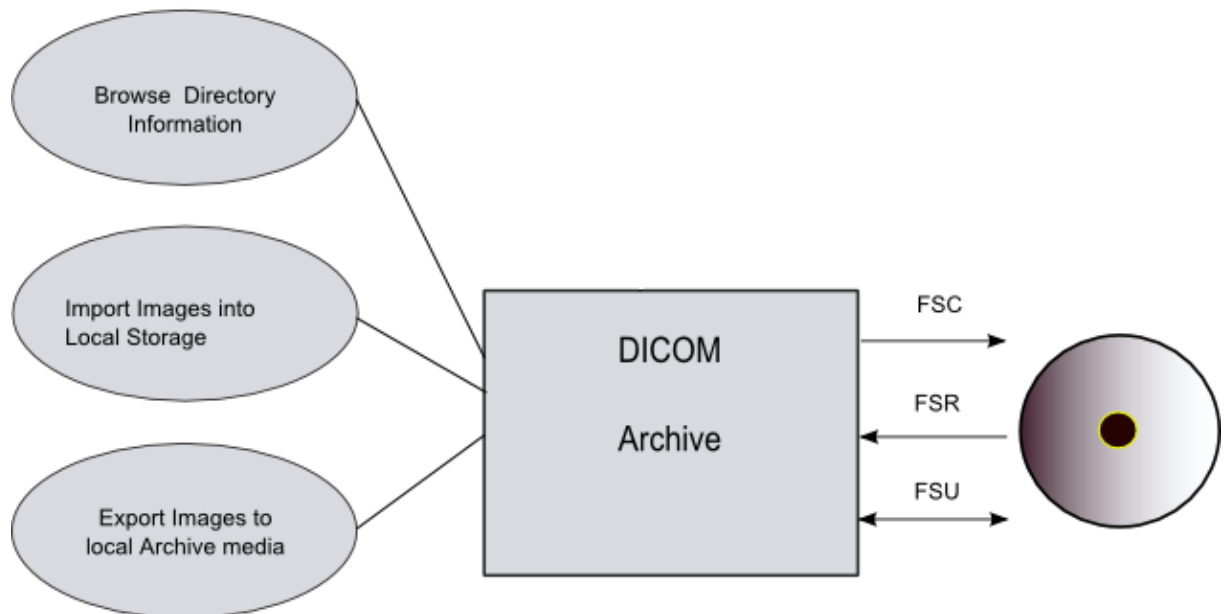


Figure 2: Application Data Flow DICOM Archive

The DICOM archive application will serve as an interface to the CD-R/DVD offline medium device.

The DICOM Archive application will support the 120mm CD-R and DVD medium.

The FSU role will update new SOP Instances only to media with pre-existing File-sets conforming to the Application Profiles supported.

The contents of the DICOMDIR will temporarily be stored in Archive-Database.

5.1.2 Functional Definitions of AEs

The syngo DICOM Offline Media Storage application consists of the DICOM Archive application entity serving all interfaces to access offline media. The DICOM Archive application is capable of

- creating a new File-set onto an unwritten medium (Export to...).
- updating an existing File-set by writing new SOP Instances onto the medium (Export to...).
- importing SOP Instances from the medium onto local storage
- reading the File-sets DICOMDIR information into temporary database and pass it to display applications.

5.1.3 Activities

5.1.3.1 Description and Sequencing of Activity FSR

The DICOM Archive application will not perform transfers until the Directory information of the DICOMDIR is completely read in and displayed in the Browser.

5.1.4 Implementation Identifying Information

For Implementation Identifying Information please refer to “Table 3 - Implementation Identifying Information” in chapter 1 [“Conformance Statement Overview”](#).

5.2 AE Specifications

5.2.1 DICOM Archive Specification

The DICOM Archive provides Standard conformance to Media Storage Service Class (Interchange Option). Details are listed in following Table:

Table 51 - Mapping of Application Profiles Supported

Application Profiles Supported	Real-World Activity	Role	SC Option
PRI-SYNGO-CD PRI-SYNGO-BD AUG-GEN-CD AUG-CTMR-CD *1 AUG-XA1K-CD *1	Browse Directory Information	FSR	Interchange
	Import into local Storage	FSR	Interchange
	Export to local Archive Media	FSC, FSU	Interchange
STD-GEN-CD STD-CTMR-CD STD-XABC-CD STD-XA1K-CD STD-US-zz-yF-xxxxxx *2	Browse Directory Information	FSR	Interchange
	Import into local Storage	FSR	Interchange

5.2.1.1 File Meta Information for the Application Entity

The Source Application Entity Title is set by configuration and is same as used for Storage provider.

5.2.1.2 Activities of DICOM Archive

5.2.1.2.1 Activity "Browse Directory Information"

The DICOM Archive application acts as FSR using the interchange option when requested to read the media directory.

The DICOM archive application will read the DICOMDIR and insert those directory entries that are valid for the application profiles supported, into a local database. The database can then be used for browsing media contents.

Note: Icon Image Sequence is also supported in DICOMDIR. But only those Icon Images with Bits Allocated (0028,0100) equal to 8 and size of 64x64 or 128x128 pixels are imported into database and are visible in the Browser.

5.2.1.2.1.1 Media Storage Application Profile

See "Table 51 - Mapping of Application Profiles Supported" in section [5.2.1](#) for the Application Profiles listed that invoke this Application Entity for the Browse Directory Information activity.

5.2.1.2.2 Activity "Import into Local Storage"

The DICOM Archive application acts as FSR using the interchange option when being requested to read SOP Instances from the medium into the local storage.

The SOP Instance(s) selected from the media directory will be copied into the local storage. Only SOP Instances, that are valid for the application profile supported and are listed as supported by the Storage SCP Conformance section (Network DCS, 5.1.3), can be retrieved from Media Storage.

For media conforming to the STD-GEN-xxx Profile the following SOP Classes will be supported as FSR:

Table 52 - STD-GEN-xxx profile supported SOP Classes

Information Object Definition	SOP Class UID	Transfer Syntax UID
CR Image	1.2.840.10008.5.1.4.1.1.1	Explicit VR Little Endian Uncompressed 1.2.840.10008.1.2.1
CT image	1.2.840.10008.5.1.4.1.1.2	Explicit VR Little Endian Uncompressed 1.2.840.10008.1.2.1
Enhanced CT Image	1.2.840.10008.5.1.4.1.1.2.1	Explicit VR Little Endian Uncompressed 1.2.840.10008.1.2.1
DX Image-For Processing	1.2.840.10008.5.1.4.1.1.1.1	Explicit VR Little Endian Uncompressed 1.2.840.10008.1.2.1
DX Image-For Presentation	1.2.840.10008.5.1.4.1.1.1.1	Explicit VR Little Endian Uncompressed 1.2.840.10008.1.2.1
IOX Image-For Processing	1.2.840.10008.5.1.4.1.1.1.3.1	Explicit VR Little Endian Uncompressed 1.2.840.10008.1.2.1
IOX Image-For Presentation	1.2.840.10008.5.1.4.1.1.1.3	Explicit VR Little Endian Uncompressed 1.2.840.10008.1.2.1
MG Image-For Processing	1.2.840.10008.5.1.4.1.1.1.2.1	Explicit VR Little Endian Uncompressed 1.2.840.10008.1.2.1
MG Image-For Presentation	1.2.840.10008.5.1.4.1.1.1.2	Explicit VR Little Endian Uncompressed 1.2.840.10008.1.2.1
MR Image	1.2.840.10008.5.1.4.1.1.4	Explicit VR Little Endian Uncompressed 1.2.840.10008.1.2.1
Enhanced MR Image	1.2.840.10008.5.1.4.1.1.4.1	Explicit VR Little Endian Uncompressed 1.2.840.10008.1.2.1
MR Spectroscopy Image	1.2.840.10008.5.1.4.1.1.4.2	Explicit VR Little Endian Uncompressed 1.2.840.10008.1.2.1
Enhanced Colored MR Image	1.2.840.10008.5.1.4.1.1.4.3	Explicit VR Little Endian Uncompressed 1.2.840.10008.1.2.1
Grayscale Softcopy Presentation State Storage	1.2.840.10008.5.1.4.1.1.11.1	Explicit VR Little Endian Uncompressed 1.2.840.10008.1.2.1
X-Ray 3D Angiographic Image Storage	1.2.840.10008.5.1.4.1.1.13.1.1	Explicit VR Little Endian Uncompressed 1.2.840.10008.1.2.1
Breast Tomosynthesis Image	1.2.840.10008.5.1.4.1.1.13.1.3	Explicit VR Little Endian Uncompressed 1.2.840.10008.1.2.1
NM Image	1.2.840.10008.5.1.4.1.1.20	Explicit VR Little Endian Uncompressed 1.2.840.10008.1.2.1
PET Image	1.2.840.10008.5.1.4.1.1.128	Explicit VR Little Endian Uncompressed 1.2.840.10008.1.2.1
RT Dose	1.2.840.10008.5.1.4.1.1.481.2	Explicit VR Little Endian Uncompressed 1.2.840.10008.1.2.1
RT Image	1.2.840.10008.5.1.4.1.1.481.1	Explicit VR Little Endian Uncompressed 1.2.840.10008.1.2.1
RT Plan	1.2.840.10008.5.1.4.1.1.481.5	Explicit VR Little Endian Uncompressed 1.2.840.10008.1.2.1
RT Structure Set	1.2.840.10008.5.1.4.1.1.481.3	Explicit VR Little Endian Uncompressed 1.2.840.10008.1.2.1
RT Beams Treatment Record	1.2.840.10008.5.1.4.1.1.481.4	Explicit VR Little Endian Uncompressed 1.2.840.10008.1.2.1
RT Brachy Treatment Record	1.2.840.10008.5.1.4.1.1.481.6	Explicit VR Little Endian Uncompressed 1.2.840.10008.1.2.1
RT Treatment Summary Record	1.2.840.10008.5.1.4.1.1.481.7	Explicit VR Little Endian Uncompressed 1.2.840.10008.1.2.1
RT Ion Plan	1.2.840.10008.5.1.4.1.1.481.8	Explicit VR Little Endian Uncompressed 1.2.840.10008.1.2.1
RT Ion Beams Treatment Record	1.2.840.10008.5.1.4.1.1.481.9	Explicit VR Little Endian Uncompressed 1.2.840.10008.1.2.1

Secondary Capture Image	1.2.840.10008.5.1.4.1.1.7	Explicit VR Little Endian Uncompressed 1.2.840.10008.1.2.1
Multi-frame Single Bit Secondary Capture Image	1.2.840.10008.5.1.4.1.1.7.1	Explicit VR Little Endian Uncompressed 1.2.840.10008.1.2.1
Multi-frame Grayscale Byte Secondary Capture Image	1.2.840.10008.5.1.4.1.1.7.2	Explicit VR Little Endian Uncompressed 1.2.840.10008.1.2.1
Multi-frame Grayscale Word Secondary Capture Image	1.2.840.10008.5.1.4.1.1.7.3	Explicit VR Little Endian Uncompressed 1.2.840.10008.1.2.1
Multi-frame True Color Secondary Capture Image	1.2.840.10008.5.1.4.1.1.7.4	Explicit VR Little Endian Uncompressed 1.2.840.10008.1.2.1
Ultrasound Image (retired)	1.2.840.10008.5.1.4.1.1.6	Explicit VR Little Endian Uncompressed 1.2.840.10008.1.2.1
Ultrasound Image	1.2.840.10008.5.1.4.1.1.6.1	Explicit VR Little Endian Uncompressed 1.2.840.10008.1.2.1
Ultrasound Multi-frame Image (retired)	1.2.840.10008.5.1.4.1.1.3	Explicit VR Little Endian Uncompressed 1.2.840.10008.1.2.1
Ultrasound Multi-frame Image	1.2.840.10008.5.1.4.1.1.3.1	Explicit VR Little Endian Uncompressed 1.2.840.10008.1.2.1
X-Ray Angiographic Image	1.2.840.10008.5.1.4.1.1.12.1	Explicit VR Little Endian Uncompressed 1.2.840.10008.1.2.1
X-Ray Radiofluoroscopic Image	1.2.840.10008.5.1.4.1.1.12.2	Explicit VR Little Endian Uncompressed 1.2.840.10008.1.2.1
12-lead ECG Waveform Storage	1.2.840.10008.5.1.4.1.1.9.1.1	Explicit VR Little Endian Uncompressed 1.2.840.10008.1.2.1
Ambulatory ECG Waveform Storage	1.2.840.10008.5.1.4.1.1.9.1.3	Explicit VR Little Endian Uncompressed 1.2.840.10008.1.2.1
Basic Voice Audio Waveform Storage	1.2.840.10008.5.1.4.1.1.9.4.1	Explicit VR Little Endian Uncompressed 1.2.840.10008.1.2.1
Cardiac Electrophysiology Waveform Storage	1.2.840.10008.5.1.4.1.1.9.3.1	Explicit VR Little Endian Uncompressed 1.2.840.10008.1.2.1
General ECG Waveform Storage	1.2.840.10008.5.1.4.1.1.9.1.2	Explicit VR Little Endian Uncompressed 1.2.840.10008.1.2.1
Hemodynamic Waveform Storage	1.2.840.10008.5.1.4.1.1.9.2.1	Explicit VR Little Endian Uncompressed 1.2.840.10008.1.2.1
CSA Non-Image	1.3.12.2.1107.5.9.1	Explicit VR Little Endian Uncompressed 1.2.840.10008.1.2.1
RAW Data Storage	1.2.840.10008.5.1.4.1.1.66	Explicit VR Little Endian Uncompressed 1.2.840.10008.1.2.1
Spatial Registration Storage	1.2.840.10008.5.1.4.1.1.66.1	Explicit VR Little Endian Uncompressed 1.2.840.10008.1.2.1
Spatial Fiducials Storage	1.2.840.10008.5.1.4.1.1.66.2	Explicit VR Little Endian Uncompressed 1.2.840.10008.1.2.1
Segmentation Storage	1.2.840.10008.5.1.4.1.1.66.4	Explicit VR Little Endian Uncompressed 1.2.840.10008.1.2.1
Surface Segmentation Storage	1.2.840.10008.5.1.4.1.1.66.5	Explicit VR Little Endian Uncompressed 1.2.840.10008.1.2.1
Basic Text SR	1.2.840.10008.5.1.4.1.1.88.11	Explicit VR Little Endian Uncompressed 1.2.840.10008.1.2.1
Enhanced SR	1.2.840.10008.5.1.4.1.1.88.22	Explicit VR Little Endian Uncompressed 1.2.840.10008.1.2.1
Comprehensive SR	1.2.840.10008.5.1.4.1.1.88.33	Explicit VR Little Endian Uncompressed 1.2.840.10008.1.2.1
Mammography CAD SR	1.2.840.10008.5.1.4.1.1.88.50	Explicit VR Little Endian Uncompressed 1.2.840.10008.1.2.1
Key Object Selection Document	1.2.840.10008.5.1.4.1.1.88.59	Explicit VR Little Endian Uncompressed 1.2.840.10008.1.2.1
Chest CAD SR	1.2.840.10008.5.1.4.1.1.88.65	Explicit VR Little Endian Uncompressed 1.2.840.10008.1.2.1
Procedure Log	1.2.840.10008.5.1.4.1.1.88.40	Explicit VR Little Endian Uncompressed 1.2.840.10008.1.2.1
X-Ray Radiation Dose SR	1.2.840.10008.5.1.4.1.1.88.67	Explicit VR Little Endian Uncompressed 1.2.840.10008.1.2.1

Encapsulated PDF	1.2.840.10008.5.1.4.1.1.104.1	Explicit VR Little Endian Uncompressed 1.2.840.10008.1.2.1
------------------	-------------------------------	---

5.2.1.2.2.1 Media Storage Application Profile

See “Table 51 - Mapping of Application Profiles Supported” in section [5.2.1](#) for the Application Profiles listed that invoke this Application Entity for the Import into Local Storage activity.

5.2.1.3 Activity “Export to Local Archive Media”

The DICOM Archive application acts as FSU (for media with existing DICOM file-set) or FSC (media not initialized) using the interchange option when requested to copy SOP Instances from the local storage to local Archive Medium.

The DICOM Archive application will receive a list of SOP Instances to be copied to the local archive medium. According to the state of the medium inserted (new medium, Medium with DICOM file-set) the validity of the SOP Instances according to the applicable profile is checked. Only valid SOP Instances are accepted.

The DICOM Archive application will not finalize the medium.

With the resizing feature of the syngo DICOM application, a copy of images in Cardiac Format (512x512, 8Bit) can be written onto medium.

5.2.1.3.1.1 Media Storage Application Profile

See “Table 51 - Mapping of Application Profiles Supported” in section [5.2.1](#) for the Application Profiles listed that invoke this Application Entity for the Export to Local Archive Media activity.

5.3 Augmented and Private Application Profiles

n.a

5.4 Media Configuration

5.4.1 Single- / Multi-Session CD burning

Please refer to most recent Service / Configuration documentation of syngo for changing between the single-session and multi-session recording modes.

5.4.2 Auto-Labeling

Please refer to most recent Service / Configuration documentation of syngo for activating the auto-labeling of CD media to avoid the label inquiry dialog when using automatic media export. The auto-labeling can be activated with the "Viewer on CD" feature being implicitly checked or not.

6 Support of Extended Character Sets

The syngo DICOM application supports the following character sets as defined in the four tables below:

Table 53 - Supported Single-Byte Character Sets (w/o Code Ext.)

Character Set Description	Defined Term	ISO registration number	Character Set
Default repertoire	none	ISO_IR 6	ISO 646:
Latin alphabet No. 1	ISO_IR 100	ISO_IR 100	Supplementary set
		ISO_IR 6	ISO 646:
Latin alphabet No. 2	ISO_IR 101	ISO_IR 101	Supplementary set
		ISO_IR 6	ISO 646
Latin alphabet No. 3	ISO_IR 109	ISO_IR 109	Supplementary set
		ISO_IR 6	ISO 646
Latin alphabet No. 4	ISO_IR 110	ISO_IR 110	Supplementary set
		ISO_IR 6	ISO 646
Cyrillic	ISO_IR 144	ISO_IR 144	Supplementary set
		ISO_IR 6	ISO 646
Arabic	ISO_IR 127	ISO_IR 127	Supplementary set
		ISO_IR 6	ISO 646
Greek	ISO_IR 126	ISO_IR 126	Supplementary set
		ISO_IR 6	ISO 646
Hebrew	ISO_IR 138	ISO_IR 138	Supplementary set
		ISO_IR 6	ISO 646
Latin alphabet No. 5	ISO_IR 148	ISO_IR 148	Supplementary set
		ISO_IR 6	ISO 646
Japanese	ISO_IR 13	ISO_IR 13	JIS X 0201: Katakana
		ISO_IR 14	JIS X 0201: Romaji

Table 54 - Supported Single-Byte Character Sets (with Code Ext.)

Character Set Description	Defined Term	Standard for Code Extension	ESC sequence	ISO registration number	Character Set
Default repertoire	ISO 2022 IR 6	ISO 2022	ESC 02/08 04/02	ISO-IR 6	ISO 646
Latin alphabet No.1	ISO 2022 IR 100	ISO 2022	ESC 02/13 04/01	ISO-IR 100	Supplementary set
		ISO 2022	ESC 02/08 04/02	ISO-IR 6	ISO 646
Latin alphabet No.2	ISO 2022 IR 101	ISO 2022	ESC 02/13 04/02	ISO-IR 101	Supplementary set
		ISO 2022	ESC 02/08 04/02	ISO-IR 6	ISO 646
Latin alphabet No.3	ISO 2022 IR 109	ISO 2022	ESC 02/13 04/03	ISO-IR 109	Supplementary set
		ISO 2022	ESC 02/08 04/02	ISO-IR 6	ISO 646
Latin alphabet No.4	ISO 2022 IR 110	ISO 2022	ESC 02/13 04/04	ISO-IR 110	Supplementary set
		ISO 2022	ESC 02/08 04/02	ISO-IR 6	ISO 646
Cyrillic	ISO 2022 IR 144	ISO 2022	ESC 02/13 04/12	ISO-IR 144	Supplementary set
		ISO 2022	ESC 02/08 04/02	ISO-IR 6	ISO 646
Arabic	ISO 2022 IR 127	ISO 2022	ESC 02/13 04/07	ISO-IR 127	Supplementary set
		ISO 2022	ESC 02/08 04/02	ISO-IR 6	ISO 646
Greek	ISO 2022 IR 126	ISO 2022	ESC 02/13 04/06	ISO-IR 126	Supplementary set
		ISO 2022	ESC 02/08 04/02	ISO-IR 6	ISO 646
Hebrew	ISO 2022 IR 138	ISO 2022	ESC 02/13 04/08	ISO-IR 138	Supplementary set
		ISO 2022	ESC 02/08 04/02	ISO-IR 6	ISO 646
Latin alphabet No.5	ISO 2022 IR 148	ISO 2022	ESC 02/13 04/13	ISO-IR 148	Supplementary set
		ISO 2022	ESC 02/08 04/02	ISO-IR 6	ISO 646
Japanese	ISO 2022 IR 13	ISO 2022	ESC 02/09 04/09	ISO-IR 13	JIS X 0201: Katakana
		ISO 2022	ESC 02/08 04/10	ISO-IR 14	JIS X 0201-1976: Romaji

Table 55 - Supported Multi-Byte Character Sets (w/o Code Ext.)

Character Set Description	Defined Term	ISO registration number	Character Set
Unicode	ISO_IR 192	ISO 10646	Unicode in UTF-8
Chinese	GB18030	GB18030	GB 18030-2000 (China Association for Standardization)

Table 56 - Supported Multi-Byte Character Sets (with Code Ext.)

Character Set Description	Defined Term	Standard for Code Extension	ESC sequence	ISO registration number	Character Set
Japanese	ISO 2022 IR 87	ISO 2022	ESC 02/04 04/02	ISO-IR 87	JIS X 0208: Kanji
	ISO 2022 IR 159	ISO 2022	ESC 02/04 02/08 04/04	ISO-IR 159	JIS X 0212: Supplementary Kanji set
Chinese ^h	ISO 2022 IR 58	ISO 2022	ESC 02/04 04/01	ISO-IR 58	GB2312-80 (China Association for Standardization)

When there is a mismatch between the Specific Character Set tag (0008,0005) and the characters in an IOD received by the system, then the following measures are taken to make the characters DICOM conform:

- Try to import with ISO_IR 100. If ISO_IR 100 fails, convert each illegal character to a '?'.

There are now three categories of character sets which have to be differentiated because of their different encoding formats:

- Conventional ISO character sets: ISO_IR 6, ISO 2022 IR 6, ISO_IR 100, etc.
→ encoded in ISO 2022
- ISO IR_192 → encoded in UTF-8
- GB18030 → encoded in GB18030

It is not possible to recognize the following mismatches automatically on receiving or importing:

- An attribute value is encoded in ISO_IR 192 ← → (0008,0005) contains a conventional ISO character set as primary character set.
- An attribute value is encoded in GB18030 ← → (0008,0005) contains a conventional ISO character set as primary character set.
- An attribute value is encoded in ISO 2022 ← → (0008,0005) contains ISO_IR 192.
- An attribute value is encoded in ISO 2022 ← → (0008,0005) contains GB18030

An IOD that contains one of the above mentioned inconsistencies is not DICOM conform. As these kinds of inconsistencies cannot be recognized by the system, the IOD will not be rejected but the character data might not be displayed as intended.

Older versions of syngo do not support the newly introduced character sets ISO_IR 192 and GB18030 and their special encodings. That means, an IOD which contains one of these new character sets in (0008,0005) will be rejected by an older syngo.

^h Note: This Character Set is an extension of DICOM for the Chinese language.

7 Security

7.1 Security Profile

syngo conforms to the IHE Basic Security Integration Profile that is used for the DICOM Communication.

syngo allows the use of either a conventional (non-secure) DICOM communication or a secure DICOM communication. For secure DICOM communication syngo application uses the Transport Layer Protocol (TLS v1.0). Following features are supported for the secure DICOM communication. The port in which syngo act as SCP for secure DICOM communication is 2762 (fixed). The port in which syngo act as SCP for unsecure DICOM communication is 104 (fixed). By default secure mode is activated and can be changed by configuration for each remote node.

Following security profiles are done in syngo using TLS 1.0 protocol:

- Secure authentication of node
- Integrity and confidentiality of transmitted data
- Generation of audit trail records access control and user authentication.

7.1.1 Security Transport Connection Profiles

syngo conforms to the Basic TLS Transport Connection Profile and initiates and accepts TLS connections with Storage Commitment.

syngo provides a Windows Certificate Store panel that allows to configure the certificate that is used for the DICOM communication. Secure communication is a “mode of operation” of syngo supported by the implementation of the DICOM Basic TLS Secure Transport Connection Profile. This functionality is used by the local and remote node to authenticate each other before they exchange DICOM information. For secure communication the TLS protocol v1.0 is used which provides message authentication, integrity and confidentiality.

syngo supports X.509 certificates. The type of X.509 certificates that are supported are:

1. Self Signed certificate
2. Chain building certificate (Trusted chain building, Trusted CA).

The following TLS certification checks will be done (TLS Handshake). The system (either server or client) that sends its certificate will:

1. Choose the certificate according to Common Name (CN), if the self signed certificate is used. If customer specific certificate needs to be used then the serial number of the certificate is used for choosing the certificate.

The server verifies:

2. that the client certificate is X.509 certificate which is not tampered with
3. that the client certificate is in the list of trusted certificates (Trust Chain Building)
4. that the client certificate is not in the revoked list

5. that the client certificate is not expired (present time is between “Valid From” and “Valid To” fields of the X.509 certificate)
6. that the client certificate has the correct purpose (at least the client authentication purpose).

The client verifies:

7. that the server certificate is a X.509 certificate which is not tampered with
8. that the server certificate is in the list of trusted certificates (Trust Chain Building)
9. that the server certificate is not in the revoked list
10. that the server certificate is not expired (present time is between “Valid From” and “Valid To” fields of the X.509 certificate)
11. that the server certificate has the correct purpose (at least the server authentication purpose).

No verification is done on certificate for:

1. Direct certificate validation
2. Certificate received from peer have multiple X.509 certificates within the TLS Handshake.

The X.509 certificate imported and used for DICOM communication must have the possibility:

1. must provide the purpose set for Client and Server Authentication
2. must be exportable to generate the certificate file and the private key file.

If intermediate and root X.509 certificates are present then the intermediate certificate must be imported to Intermediate Certificate Authorities→Certificates. The root certificate must be imported to the Trusted Root Certificates→Certificates.

syngo communicates with either of the following Cipher suites for encrypting the data send across the network:

- TLS_RSA_WITH_AES_128_CBC_SHA
- TLS_RSA_WITH_3DES_EDE_CBC_SHA

Note: syngo provides no support for NULL Cipher (TLS_RSA_WITH_NULL_SHA).

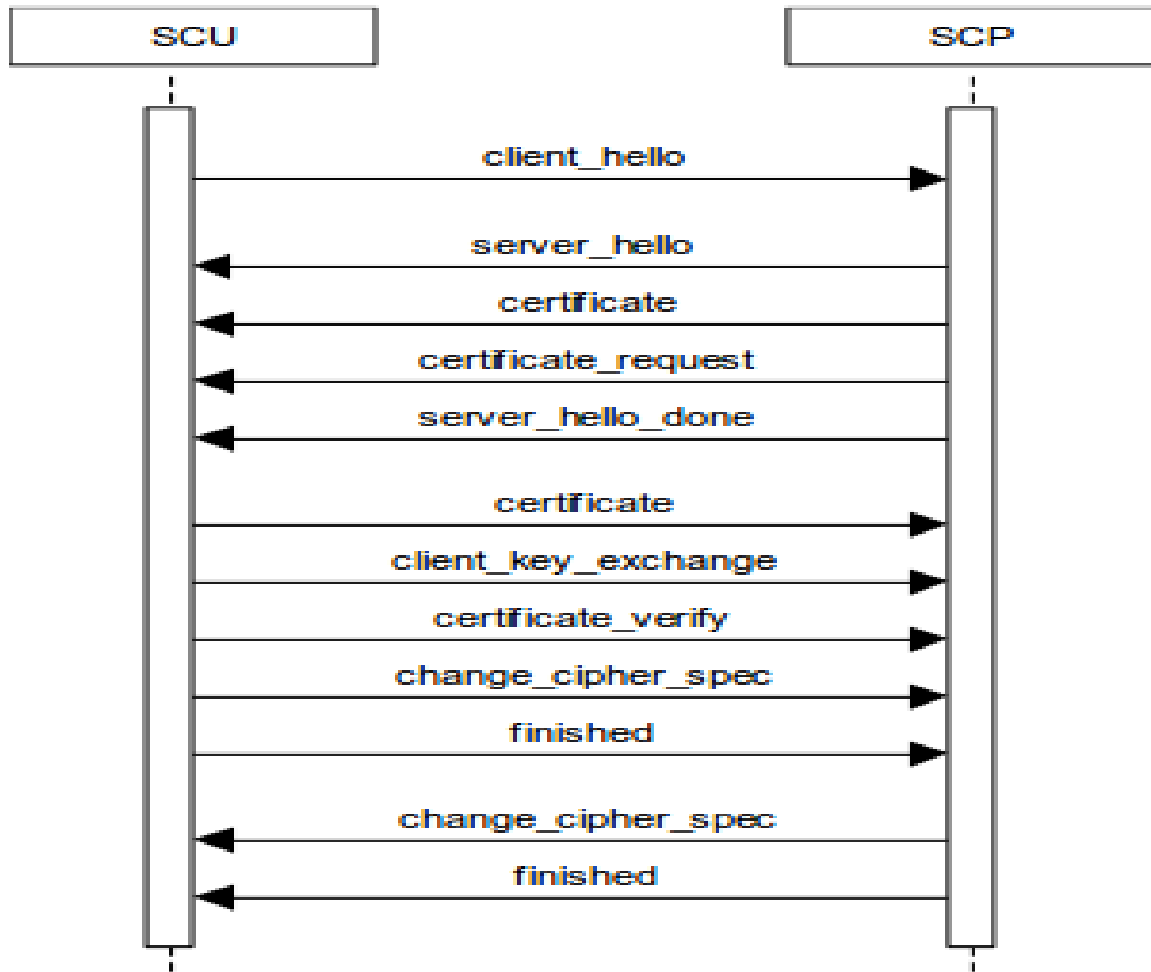


Figure 3: TLS Handshake Message Protocol

8 Annexes

8.1 MR Image IOD

8.1.1 Patient Module

Attribute Name	Tag	Supported Values
Patient's Name	0010,0010	set by registration or worklist; used for image annotation
Patient ID	0010,0020	set by registration or worklist; used for image annotation
Patient's Birth Date	0010,0030	set by registration or worklist; used for image annotation
Patient's Sex	0010,0040	set by registration or worklist
Other Patient IDs	0010,1000	
Other Patient Names	0010,1001	
Ethnic Group	0010,2160	set by worklist
Patient Comments	0010,4000	set by worklist

8.1.2 General Study Module

Attribute Name	Tag	Supported Values
Study Instance UID	0020,000D	set by internal data base or worklist
Study Date	0008,0020	set by acquisition
Study Time	0008,0030	set by acquisition
Referring Physician's Name	0008,0090	set by registration or worklist
Study ID	0020,0010	set by internal data base; used for image annotation
Accession Number	0008,0050	set by registration or worklist
Study Description	0008,1030	set by registration user interface
Procedure Code Sequence	0008,1032	set by mpps
> Code Value	0008,0100	set by mpps
> Code Scheme Designator	0008,0102	set by mpps
> Code Meaning	0008,0104	set by mpps

8.1.3 Patient Study Module

Attribute Name	Tag	Supported Values
Admitting Diagnoses Description	0008,1080	set by acquisition user interface
Patient's Age	0010,1010	set by registration or worklist
Patient's Size	0010,1020	set by registration or worklist
Patient's Weight	0010,1030	set by registration or worklist

8.1.4 General Series Module

Attribute Name	Tag	Supported Values
Modality	0008,0060	MR
Series Instance UID	0020,000E	set by internal data base
Series Number	0020,0011	set by internal data base; used for image annotation
Series Date	0008,0021	set by acquisition
Series Time	0008,0031	set by acquisition
Performing Physicians' Name	0008,1050	set by registration user interface
Protocol Name	0018,1030	set by acquisition
Series Description	0008,103E	set by acquisition
Operators' Name	0008,1070	set by registration user interface
Referenced Performed Procedure Step Sequence	0008,1111	identifies Modality Performed Procedure Step related to the series
> Referenced SOP Class UID		identifies Modality Performed SOP Class related to the series
> Referenced SOP Instance UID		identifies Modality Performed SOP Instance UID related to the series
Body Part Examined	0018,0015	set by acquisition user interface
Patient Position	0018,5100	set by registration user interface; used for image annotation
Request Attributes Sequence	0040,0275	set by worklist (not available with all post-processing applications)
> Requested Procedure ID	0040,1001	set by worklist (not available with all post-processing applications)
> Requested Procedure Description	0032,1060	set by worklist (not available with all post-processing applications)
> Scheduled Procedure Step ID	0040,0009	set by worklist (not available with all post-processing applications)
> Scheduled Procedure Step Description	0040,0007	set by worklist (not available with all post-processing applications)
> Scheduled Procedure Code Sequence	0040,0008	set by worklist (not available with all post-processing applications)
>> Code Value	0008,0100	set by worklist (not available with all post-processing applications)
>> Code Scheme Designator	0008,0102	set by worklist (not available with all post-processing applications)
>> Code Scheme Version	0008,0103	set by worklist (not available with all post-processing applications)
>> Code Meaning	0008,0104	set by worklist (not available with all post-processing applications)
Performed Procedure Step ID	0040,0253	copied from scheduled procedure step id (not available with all post-processing applications)
Performed Procedure Step Start Date	0040,0244	set by acquisition (not available with all post-processing applications)
Performed Procedure Step Start Time	0040,0245	set by acquisition (not available with all post-processing applications)
Performed Procedure Step Description	0040,0254	copied from scheduled procedure step description

		(not available with all post-processing applications)
--	--	---

8.1.5 Frame of Reference Module

Attribute Name	Tag	Supported Values
Frame of Reference UID	0020,0052	set by acquisition
Position Reference Indicator	0020,1040	set by acquisition

8.1.6 General Equipment Module

Attribute Name	Tag	Supported Values
Manufacturer	0008,0070	SIEMENS
Institution Name	0008,0080	set by configuration; used for image annotation
Institution Address	0008,0081	Street number, Street, City, District, Zip Code, Country
Station Name	0008,1010	hostname; set by configuration
Manufacturer's Model Name	0008,1090	set by configuration; used for image annotation
Device Serial Number	0018,1000	set by configuration
Software Versions	0018,1020	used for image annotation

8.1.7 General Image Module

Attribute Name	Tag	Supported Values
Instance Number	0020,0013	set by internal data base; used for image annotation
Content Date	0008,0023	set by acquisition
Content Time	0008,0033	set by acquisition
Image Type	0008,0008	values might be set by acquisition and post-processing applications and may reflect the processing history
Acquisition Number	0020,0012	set by acquisition
Acquisition Date	0008,0022	set by acquisition; used for image annotation
Acquisition Time	0008,0032	set by acquisition; used for image annotation
Referenced Image Sequence	0008,1140	set by Graphical Slice Position
> Referenced SOP Class UID	0008,1150	set by Graphical Slice Position
> Referenced SOP Instance UID	0008,1155	set by Graphical Slice Position
Derivation Description	0008,2111	set by applications which derived images
Source Image Sequence	0008,2112	set by applications which derived images
> Referenced SOP Class UID	0008,1150	set by applications which derived images
> Referenced SOP Instance UID	0008,1155	set by applications which derived images

Image Comments	0020,4000	set by registration and acquisition user interface; used for image annotation
----------------	-----------	--

8.1.8 Image Plane Module

Attribute Name	Tag	Supported Values
Pixel Spacing	0028,0030	set by acquisition
Image Orientation	0020,0037	set by acquisition; used for image annotation
Image Position	0020,0032	set by acquisition; used for image annotation
Slice Thickness	0018,0050	set by acquisition; used for image annotation
Slice Location	0020,1041	set by acquisition; accumulated from image orientation and image position and used as term SP in the image annotation

8.1.9 Image Pixel Module

Attribute Name	Tag	Supported Values
Samples per Pixel	0028,0002	1
Photometric Interpretation	0028,0004	MONOCHROME2
Rows	0028,0010	set by acquisition
Columns	0028,0011	set by acquisition
Bits Allocated	0028,0100	16
Bits Stored	0028,0101	12
High Bit	0028,0102	11
Pixel Representation	0028,0103	0
Pixel Data	7FE0,0010	set by acquisition
Smallest Image Pixel Value	0028,0106	set by acquisition
Largest Image Pixel Value	0028,0107	set by acquisition

8.1.10 Contrast/Bolus Module

Attribute Name	Tag	Supported Values
Contrast/Bolus Agent	0018,0010	set by acquisition contrast user interface; used for image annotation
Contrast/Bolus Agent Sequence	0018,0012	set by acquisition contrast user interface
> Code Value	0008,0100	set by acquisition contrast user interface
> Code Scheme Designator	0008,0102	99SDM
Contrast/Bolus Volume	0018,1041	set by acquisition contrast user interface.
Contrast/Bolus Total Dose	0018,1044	set by acquisition contrast user interface.
Contrast Flow Duration(s)	0018,1047	set by acquisition contrast user interface.
Contrast/Bolus Ingredient	0018,1048	set by acquisition contrast user interface. Defined

		Terms: IODINE GADOLINIUM CARBON DIOXIDE BARIUM
Contrast/Bolus Ingredient Concentration	0018,1049	set by acquisition contrast user interface.

8.1.11 MR Image Module

Attribute Name	Tag	Supported Values
Image Type	0008,0008	set by acquisition/applications; used for image annotation
Samples per Pixel	0028,0002	1
Photometric Interpretation	0028,0004	MONOCHROME2
Bits Allocated	0028,0100	16
Scanning Sequence	0018,0020	set by acquisition
Sequence Variant	0018,0021	set by acquisition
Scan Options	0018,0022	set by acquisition; used for image annotation
MR Acquisition Type	0018,0023	set by acquisition
Repetition Time	0018,0080	set by acquisition; used for image annotation
Echo Time	0018,0081	set by acquisition; used for image annotation
Echo Train Length	0018,0091	set by acquisition
Inversion Time	0018,0082	set by acquisition; used for image annotation
Trigger Time	0018,1060	set by acquisition; used for image annotation
Sequence Name	0018,0024	set by acquisition; used for image annotation
Angio Flag	0018,0025	set by acquisition
Number of Averages	0018,0083	set by acquisition
Imaging Frequency	0018,0084	set by acquisition
Imaged Nucleus	0018,0085	set by acquisition
Echo Number	0018,0086	set by acquisition
Magnetic Field Strength	0018,0087	set by acquisition
Spacing Between Slices	0018,0088	set by acquisition
Number of Phase Encoding Steps	0018,0089	set by acquisition
Percent Sampling	0018,0093	set by acquisition
Percent Phase Field of View	0018,0094	set by acquisition
Pixel Bandwidth	0018,0095	set by acquisition
Nominal Interval	0018,1062	set by ECG acquisition
Cardiac Number of Images	0018,1090	set by ECG acquisition
Transmitting Coil	0018,1251	set by acquisition
Acquisition Matrix	0018,1310	set by acquisition
Phase Encoding Direction	0018,1312	set by acquisition
Flip Angle	0018,1314	set by acquisition; used for image annotation
SAR	0018,1316	set by acquisition

Variable Flip Angle Flag	0018,1315	N
dB/dt	0018,1318	set by conditional implant acquisition of MAG-NETOM Aera

8.1.12 MR Private Diffusion Module

Attribute Name	Tag	VR	VM	Supported Values
Owner code of the module	0019,0010	LO	1	SIEMENS MR HEADER
Diffusion b- value	0019,xx0C	IS	1	Diffusion b-value of this particular image
Diffusion Directionality	0019,xx0D	CS	1	Diffusion directionality of this particular image
Diffusion Gradient Direction	0019,xx0E	FD	3	Diffusion gradient vector of this particular image
Diffusion b-matrix	0019,xx27	FD	6	Diffusion b-matrix encoding of this particular image

8.1.13 VOI LUT Module

Attribute Name	Tag	Supported Values
Window Center	0028,1050	set by acquisition; used for image annotation
Window Width	0028,1051	set by acquisition; used for image annotation
Window Center & Width Explanation	0028,1055	set by acquisition

8.1.14 SOP Common Module

Attribute Name	Tag	Supported Values
SOP Class UID	0008,0016	MR Storage SOP Class UID
SOP Instance UID	0008,0018	set by internal data base
Specific Character Set	0008,0005	set by configuration or worklist
Instance Creation Date	0008,0012	date the SOP instance was created
Instance Creation Time	0008,0013	time the SOP instance was created

8.2 MR Spectroscopy IOD

8.2.1 Patient Module

Attribute Name	Tag	Supported Values
Patient's Name	0010,0010	set by registration or worklist; used for image annotation
Patient ID	0010,0020	set by registration or worklist; used for image annotation
Patient's Birth Date	0010,0030	set by registration or worklist; used for image annotation

Patient's Sex	0010,0040	set by registration or worklist
---------------	-----------	---------------------------------

8.2.2 General Study Module

Attribute Name	Tag	Supported Values
Study Instance UID	0020,000D	set by internal data base or worklist
Study Date	0008,0020	set by acquisition
Study Time	0008,0030	set by acquisition
Referring Physician's Name	0008,0090	set by registration or worklist
Study ID	0020,0010	set by internal data base; used for image annotation
Accession Number	0008,0050	set by registration or worklist

8.2.3 General Series Module

Attribute Name	Tag	Supported Values
Modality	0008,0060	MR
Series Instance UID	0020,000E	set by internal data base
Series Number	0020,0011	set by internal data base; used for image annotation
Series Date	0008,0021	set by acquisition
Series Time	0008,0031	set by acquisition
Series Description	0008,103E	set by acquisition
Patient Position	0018,5100	set by registration user interface; used for image annotation

8.2.4 MR Series Module

Attribute Name	Tag	Supported Values
Modality	0008,0060	MR

8.2.5 Frame of Reference Module

Attribute Name	Tag	Supported Values
Frame of Reference UID	0020,0052	set by acquisition
Position Reference Indicator	0020,1040	empty

8.2.6 General Equipment Module

Attribute Name	Tag	Supported Values
Manufacturer	0008,0070	SIEMENS
Institution Name	0008,0080	set by configuration

8.2.7 Enhanced General Equipment Module

Attribute Name	Tag	Supported Values
Manufacturer	0008,0070	SIEMENS

8.2.8 Shared Functional Groups

Functional Group Macro	Attribute Name	Tag	Supported Values
Pixel Measures	Pixel Measure Sequence	0028,9110	supported
	>Slice Thickness	0018,0050	supported
	>Pixel Spacing	0028,0030	supported
Plane Orientation	Plane Orientation Sequence	0020,9116	supported
	>Image Orientation (Patient)	0020,0037	supported
Referenced Image	Referenced Image Sequence	0008,1140	supported
	>Purpose of Referenced Code Sequence	0040,A170	supported
	>>Code Value	0008,0100	121311
	>>Coding Scheme Designator	0008,0102	DCM
	>>Coding Scheme Version	0008,0103	not supported
	>>Code Meaning	0008,0104	Localizer
Derivation Image	Derivation Image Sequence	0008,9124	not supported
	>Derivation Description	0008,2111	not supported
	>Derivation Code Sequence	0008,9215	not supported
	>Source Image Sequence	0008,2112	not supported
	>>Purpose of Referenced Code Sequence	0040,A170	not supported
Frame Anatomy	Frame Anatomy Sequence	0020,9071	supported
	>Frame Laterality	0020,9072	U
	>Anatomic Region Sequence	0008,2218	empty
MR Spectroscopy Frame Type	MR Spectroscopy Frame Type Sequence	0018,9227	supported
	>Frame Type	0008,9007	ORIGINAL\PRIMARY\ SPECTROSCOPY\NONE
	>Volumetric Properties	0008,9206	VOLUME
	>Volume Based Calculation Technique Complex	0008,9207	NONE
	>Complex Image Component	0008,9208	COMPLEX
	>Acquisition Contrast	0008,9209	UNKNOWN
MR Timing and Related Parameters	MR Timing and Related Parameters Sequence	00189112	Supported
	>Repetition Time	0018,0080	supported
	>Flip Angle	0018,1314	supported
	>Echo Train Length	0018,0091	supported
	>RF Echo Train Length	0018,9240	1
	>Gradient Echo Train Length	0018,9241	0
	>Specific Absorption Rate Sequence	0018,9239	supported
	>>Specific Absorption Rate Definition	0018,9179	IEC_WHOLE_BODY
	>>Specific Absorption Rate Value	0018,9181	supported
	>Gradient Output Type	0018,9180	not supported
	>Gradient Output	0018,9182	not supported
	Operation Mode Sequence	0018,9176	supported
	>>Operating Mode Type	0018,9177	GRADIENT, RF, STATIC FIELD
	>>Operating Mode	0018,9178	IEC_NORMAL, IEC_FIRST_LEVEL,

			IEC SECOND LEVEL
MR Spectroscopy FOV/Geometry	MR Spectroscopy FOV/Geometry Sequence	0018,9103	supported
	Spectroscopy Acquisition Data Columns		
	Spectroscopy Acquisition Phase Rows	0018,9127	supported
	Spectroscopy Acquisition Phase Columns	0018,9095	supported
	Spectroscopy Acquisition Out-of-Plane Phase Steps	0018,9159	supported
	Percent Sampling	0018,0093	100.0
	Percent Phase Field of View	0018,0094	supported
MR Echo	MR Echo Sequence	0018,9114	supported
	>Effective Echo Time	0018,9082	supported
MR Modifier	MR Modifier Sequence	0018,9115	supported
	>Inversion Recovery	0018,9009	NO
	>Flow Compensation	0018,9010	NONE
	>T2 Preparation	0018,9021	NO
	>Spectrally Selected Excitation	0018,9026	NONE
	>Spatial Pre-saturation	0018,9027	NONE
	>Partial Fourier	0018,9081	NO
>Parallel Acquisition	0018,9077	NO	
MR Receive Coil	MR Receive Coil Sequence	0018,9042	supported
	>Receive Coil Name	0018,1250	supported
	>Receive Coil Manufacturer Name	0018,9041	supported
	>Receive Coil Type	0018,9043	MULTICOIL
	>Quadrature Receive Coil	0018,9044	supported
	>Multi-Coil Definition Sequence	0018,9045	supported
	>>Multi-Coil Element Name	0018,9047	supported
	>>Multi-Coil Element Used	0018,9048	supported
	>Multi-Coil Configuration	0018,9046	supported
MR Transmit Coil	MR Transmit Coil Sequence	0018,9049	supported
	>Transmit Coil Name	0018,1251	supported
	>Transmit Coil Manufacturer Name	0018,9050	supported
	>Transmit Coil Type	0018,9051	supported
MR Averages	MR Averages Sequence	00189119	supported
	>Number of Averages	0018,0083	supported
MR Spatial Saturation	MR Spatial Saturation Sequence	0018,9107	supported
	>Slab Thickness	0018,9104	supported
	>Slab Orientation	0018,9105	supported
	>Mid Slab Position	0018,9106	supported

8.2.9 Per-frame Functional Groups

Functional Group Macro	Attribute Name	Tag	Supported Values
Frame Content	Frame Content Sequence	00209111	supported
	>Frame Acquisition Number	0020,9156	1
	>Frame Reference Datetime	0018,9151	supported
	>Frame Acquisition Datetime	0018,9074	supported
	>Frame Acquisition Duration	0018,9220	supported
Plane Position	Plane Position Sequence	00209113	supported
	>Image Position (Patient)	0020,0032	supported

Cardiac Trigger	Cardiac Trigger Sequence	00189118	supported
	>Trigger Delay Time	0020,9153	supported

8.2.10 Multi-Frame Functional Groups Module

Attribute Name	Tag	Supported Values
Instance Number	0020,0013	supported
Content Date	0008,0023	supported
Content Time	0008,0033	supported
Number of Frames	0028,0008	supported

8.2.11 Multi-frame Dimension Module

Attribute Name	Tag	Supported Values
Dimension Organization Sequence	0020,9221	empty
Dimension Index Sequence	0020,9222	empty

8.2.12 Acquisition Context Module

Attribute Name	Tag	Supported Values
Acquisition Context Sequence	0040,0555	empty

8.2.13 MR Spectroscopy Module

Attribute Name	Tag	Supported Values
Acquisition Number	0020,0012	supported
Acquisition Datetime	0018,002A	supported
Acquisition Duration	0018,9073	supported
Referenced Image Evidence Sequence	0008,9092	supported
Content Qualification	0018,9004	PRODUCT
Resonant Nucleus	0018,9100	supported
k-space Filtering	0018,0087	supported
Magnetic Field Strength	0018,9100	supported
Applicable Safety Standard Agency	0018,9174	supported
Image Type	0008,0008	ORIGINAL/PRIMARY/SPECTROSCOPY/NONE
Volumetric Properties	0008,9206	VOLUME
Volume Based Calculation Technique Complex	0008,9207	NONE
Complex Image Component	0008,9208	COMPLEX
Acquisition Contrast	0008,9209	UNKNOWN
Transmitter Frequency	0018,9098	supported
Spectral Width	0018,9052	supported
Chemical Shift Reference	0018,9053	supported
Volume Localisation Technique	0018,9054	supported
Volume Localization Sequence	0018,9126	supported
>Slab Thickness	0018,9104	supported
>Slab Orientation	0018,9105	supported
>Mid SlabPosition	0018,9106	supported

De-coupling	0018,9059	supported
De-Coupling Nucleus	00189060	supported
DeCoupling Frequency	0018,9061	supported
De-Coupling Method	0018,9062	supported
De-CouplingChemicalShiftReference	0018,9063	4.7
Time Domain Filtering	00189065	NONE
Number Of Zero Fills	0018,9066	0
Baseline Correction	0018,9067	NONE
Frequency Correction	0018,9101	NO
First Order Phase Correction	0018,9198	NO
Water Referenced Phase Correction	0018,9199	NO

8.2.14 Cardiac Synchronization Module

Attribute Name	Tag	Supported Values
Cardiac Synchronization Technique	0018,9037	supported
Cardiac Signal Source	0018,9085	supported
Cardiac RR Interval Specified	0018,9070	supported
Cardiac Beat Rejection Technique	0018,9169	not supported
Low R-R Value	0018,1081	not supported
High R-R Value	0018,1082	not supported
Intervals Acquired	0018,1083	supported
Intervals Rejected	0018,1084	supported

8.2.15 MR Spectroscopy Pulse Sequence Module

Attribute Name	Tag	Supported Values
Pulse Sequence Name	0018,9005	supported
MR Spectroscopy Acquisition Type	0018,9200	supported
Echo Pulse Sequence	0018,9008	SPIN
Multi Spin Echo	0018,9011	NO
Multi-planar Excitation	0018,9012	NO
Steady State Pulse Sequence	0018,9017	NONE
Echo Planar Pulse Sequence	0018,9018	NO
Spectrally Selected Suppression	0018,9025	supported
Geometry of k-Space Traversal	0018,9032	RECTILINEAR
Rectilinear Phase Encode Reordering	0018,9034	LINEAR
Segmented k-Space Traversal	0018,9033	SINGLE
Coverage of k-Space	0018,9094	supported
Number of k-Space Trajectories	0018,9093	1

8.2.16 MR Spectroscopy Data Module

Attribute Name	Tag	Supported Values
Rows	0028,0010	supported
Columns	0028,0011	supported
Data Point Rows	0028,9001	1

Data Point Columns	0028,9002	supported
Data Representation	0028,9108	COMPLEX
Signal Domain Columns	0028,9003	TIME
Signal Domains Rows	0028,9235	supported
Spectroscopy Data	5600,0020	supported

8.2.17 SOP Common Module

Attribute Name	Tag	Supported Values
SOP Class UID	0008,0016	MR Spectroscopy SOP Class UID
SOP Instance UID	0008,0018	set by internal data base
Specific Character Set	0008,0005	set by configuration or worklist

8.3 MR Evidence Document Templates

The results of evidence document creation applications are written to the content sequence of a structured evidence document. The content of such an evidence document is specified in a template. The definition of the templates is described in a separate documentation if it is not specified by the DICOM Standard Part 16. A copy of this document could be ordered.

Examples of these applications are:

- Cardiac evaluation
- Vascular evaluation
- Mean curve evaluation
- PhoenixZip documentation.

8.4 SIEMENS Private Non-Image IOD

For encoding binary data-streams not representing image data, Siemens has created a private "Non-Image IOD" according to the rules governed by the DICOM Standard. The following section will roll-out the definition of this Private IOD. It can be communicated with Network Storage Service and Offline Media Storage Services.

The Siemens "Non-Image IOD" is identified by a private Non-Image Storage SOP Class UID of

„1.3.12.2.1107.5.9.1“

8.4.1 Siemens Non-Image IOD – E-R Model

The E-R model in A.1.2 depicts those components of the DICOM Information Model which directly refer to the Siemens Non-Image IOD. The Frame of Reference IE, Overlay IE, Modality Lookup-Table IE, VOI Lookup-Table IE and Curve IE are not components of the Siemens Non-Image IOD.

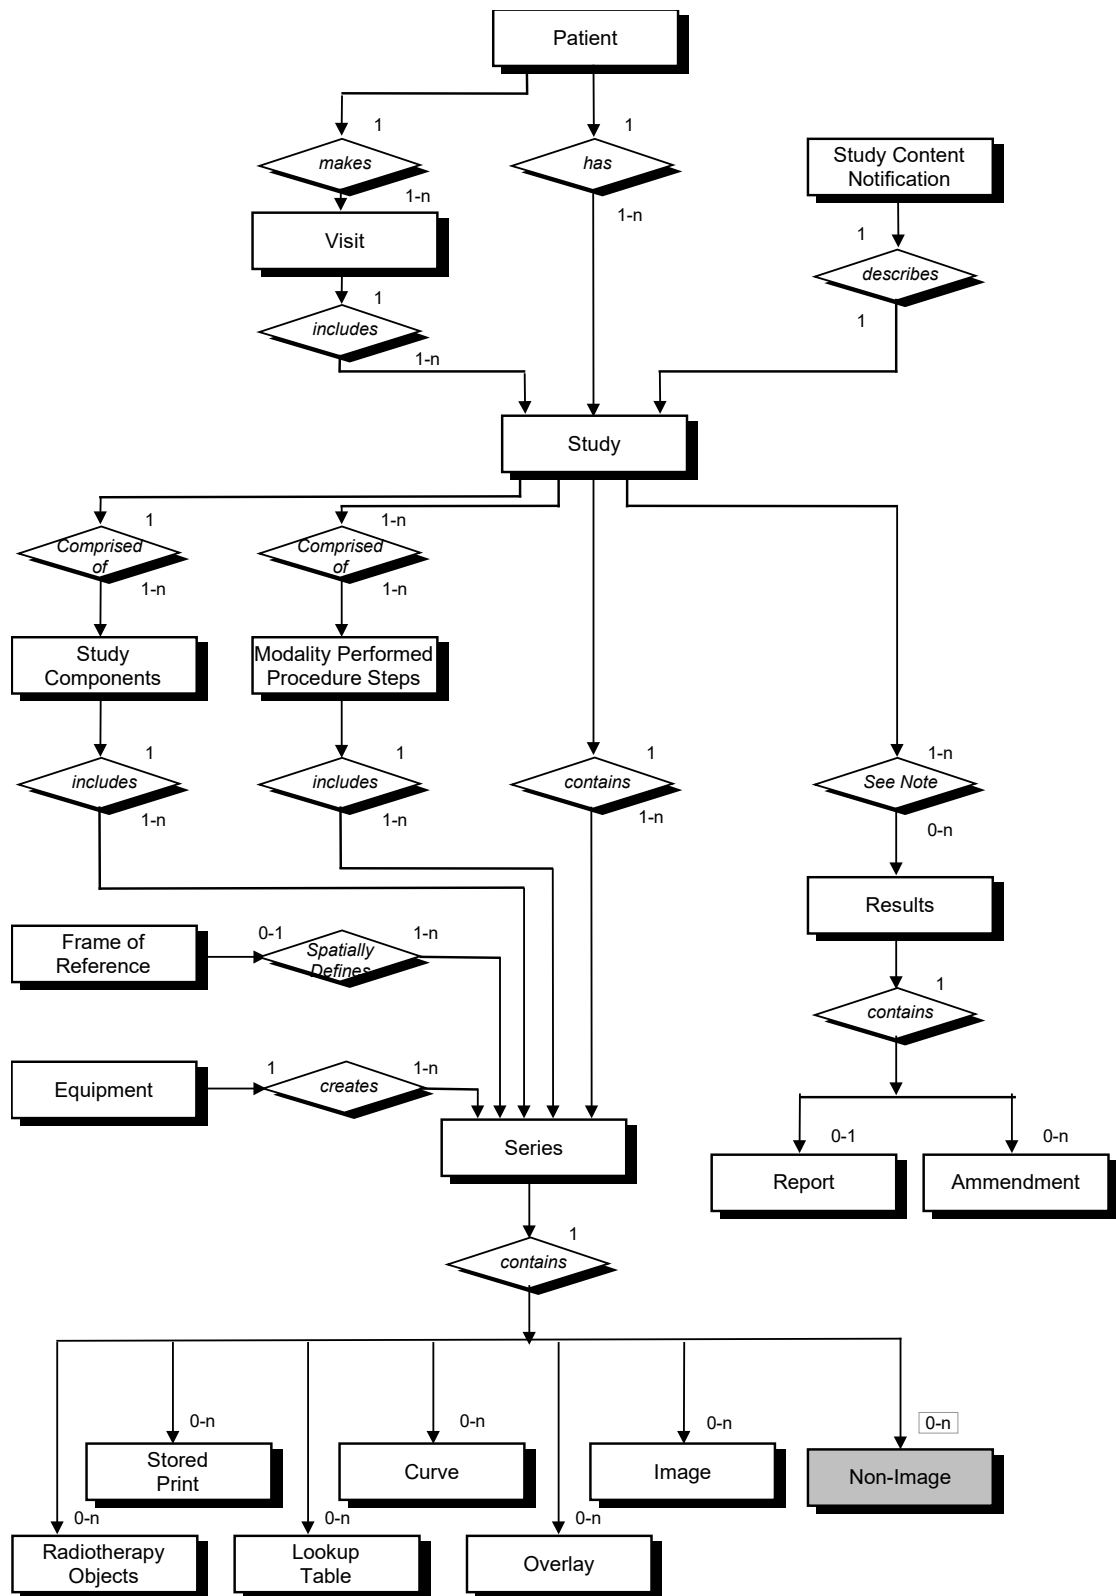


Figure 4: Siemens Non-Image IOD – E-R Model

8.4.2 Siemens Non-Image IOD - Module Table

Table 57 - Siemens Non-Image IOD - Module Table

IE	Module	Reference	Usage
Patient	Patient	[1] PS3.3 C.7.1.1	M
Study	General Study	[1] PS3.3 C.7.2.1	M
	Patient Study	[1] PS3.3 C.7.2.2	U
Series	General Series	[1] PS3.3 C.7.3.1	M
Equipment	General Equipment	[1] PS3.3 C.7.5.1	U
CSA	CSA Image Header	A.2.1	U
	CSA Series Header	A.2.2	U
	MEDCOM Header	A.2.3	U
	CSA Non-Image	A.1.3.1	M
	SOP Common	[1] PS3.3 C.12.1	M

8.4.3 CSA Series Header Module

Table 58 - private IOD Attributes that describe the CSA Series Header:

Attribute Name	Tag	Owner	Type	Notes
CSA Series Header Type	(0029,xx18)	SIEMENS CSA HEADER	1	CSA Series Header identification characteristics. Defined Terms: NUM 4 = NUMARIS/4
CSA Series Header Version	(0029,xx19)	SIEMENS CSA HEADER	3	Version of CSA Series Header Info (0029,xx20) format.
CSA Series Header Info	(0029,xx20)	SIEMENS CSA HEADER	3	Manufacturer model dependent information.

8.4.4 Siemens Non-Image IOD - Modules

8.4.4.1 CSA Non-Image Module

Table 59 Private IOD Attributes that describe CSA Non-Images.

Attribute Name	Tag	Owner	Type	Notes
Image Type	(0008,0008)	-	3	Image identification characteristics.
Acquisition Date	(0008,0022)	-	3	The date the acquisition of data that resulted in this data set started.
Acquisition Time	(0008,0032)	-	3	The time the acquisition of data that resulted in this data set started.
Conversion Type	(0008,0064)	-	3	Describes the kind of image conversion. Defined Terms: DV = Digitized Video, DI = Digital Interface, DF = Digitized Film, WSD = Workstation.
Referenced Image Sequence	(0008,1140)	-	3	A sequence which provides reference to a set of Image SOP Class/Instance identifying other images significantly related to this data set. Encoded as sequence of items: (0008,1150) and (0008,1155).
Derivation Description	(0008,2111)	-	3	A text description of how this data set was derived.
Source Image Sequence	(0008,2112)	-	3	A Sequence which identifies the set of Image SOP Class/Instance pairs of the Images which were used to

				derive this data set. Zero or more Items may be included in this Sequence. Encoded as sequence of items: (0008,1150) and (0008,1155).
Patient Position	(0018,5100)	-	3	Patient position descriptor relative to the equipment.
Acquisition Number	(0020,0012)	-	3	A number identifying the single continuous gathering of data over a period of time which resulted in this data set.
Image Number	(0020,0013)	-	3	A number that identifies this data set.
Frame of Reference UID	(0020,0052)	-	3	Uniquely identifies the frame of reference for a Series.
Image Comments	(0020,4000)	-	3	User-defined comments about the image.
Quality Control Image	(0028,0300)	-	3	Indicates whether or not this image is a quality control or phantom image. If this Attribute is absent, then the image may or may not be a quality control or phantom image. Enumerated Values: YES, NO.
Burned in Annotation	(0028,0301)	-	3	Indicates whether or not image contains sufficient burned in annotation to identify the patient and date the image was acquired. If this Attribute is absent, then the image may or may not contain burned in annotation. Enumerated Values: YES, NO.
Lossy Image Compression	(0028,2110)	-	3	Specifies whether an Image has undergone lossy compression. Enumerated Values: 00 = Image has NOT been subjected to lossy compression, 01 = Image has been subjected to lossy compression.
Lossy Image Compression Ratio	(0028,2112)	-	3	Describes the approximate lossy compression ratio(s) that have been applied to this image. May be multi valued if successive lossy compression steps have been applied.
CSA Data Type	(0029,xx08)	SIEMENS CSA NON-IMAGE	1	CSA Data identification characteristics. Defined Terms: BSR REPORT = Study Report Data 3D EDITOR 3D FLY PATH = Fly Through Data 3D FLY VRT = Fly Through Data 3D FUSION MATRIX = Fusion Data RAW DATA NUM 4 = NUMARIS/ Raw Data RAW DATA SOM 5 = SOMARIS/ Raw Data RT3D CONFIG = InSpaceIS Data SPEC NUM 4 = NUMARIS/4 Spectroscopy
CSA Data Version	(0029,xx09)	SIEMENS CSA NON-IMAGE	3	Version of CSA Data Info (0029,xx10) format and CSA Non-Image Data (7FE1,xx10) format.
CSA Data Info	(0029,xx10)	SIEMENS CSA NON-IMAGE	3	Information to describe the CSA Data (7FE1,xx10).
CSA Data	(7FE1,xx10)	SIEMENS CSA NON-IMAGE	2	Binary data as byte stream.

8.5 Siemens Standard Extended Modules

Table 60 - Siemens Standard Extended Modules

IE	Module	Reference	Usage	Note
Image	CSA Image Header	8.2.1	U	private GG information
	CSA Series Header	8.2.2	U	
	MEDCOM Header	8.2.3	U	private syngo information
	MEDCOM OOG	8.2.4	U	if object graphics is attached to image

8.5.1 CSA Image Header Module

Table 61 - private IOD Attributes that describe the CSA Image Header:

Attribute Name	Tag	Owner	Type	Notes
CSA Image Header Type	(0029,xx08)	SIEMENS CSA HEADER	1	CSA Image Header identification characteristics. Defined Terms: NUM 4 = NUMARIS/4 SOM 5 = SOMARIS/5
CSA Image Header Version	(0029,xx09)	SIEMENS CSA HEADER	3	Version of CSA Image Header Info (0029,xx10) format.
CSA Image Header Info	(0029,xx10)	SIEMENS CSA HEADER	3	Manufacturer model dependent information.

8.5.2 MEDCOM Header Module

Table 62 - private IOD Attributes that describe MEDCOM Header:

Attribute Name	Tag	Owner	Type	Notes
MedCom Header Type	(0029,xx08)	SIEMENS MEDCOM HEADER	1C	MedCom Header identification characteristics. Defined Terms: MEDCOM 1 (Required if MedCom Header Info (0029,xx10) present.)
MedCom Header Version	(0029,xx09)	SIEMENS MEDCOM HEADER	2C	Version of MedCom Header Info (0029,xx10) format. (Required if MEDCOM Header Info (0029,xx10) present.)
MedCom Header Info	(0029,xx10)	SIEMENS MEDCOM HEADER	3	Manufacturer model dependent information. The value of the attribute MedCom Header Info (0029,xx10) can be build up in each user defined format.
MedCom History Information	(0029,xx20)	SIEMENS MEDCOM HEADER	3	MedCom defined Patient Registration history information. See A.2.3.1.
Application Header Sequence	(0029,xx40)	SIEMENS MEDCOM HEADER	3	Sequence of Application Header items. Zero or more items are possible.
>Application Header Type	(0029,xx41)	SIEMENS MEDCOM HEADER	1C	Application Header identification characteristics. Required, if Sequence is sent.
>Application Header ID	(0029,xx42)	SIEMENS MEDCOM HEADER	3	Identification of an application header
>Application Header Version	(0029,xx43)	SIEMENS MEDCOM HEADER	3	Version of CSA Series Header Info (0029,xx44) format.

>Application Header Info	(0029,xx44)	SIEMENS HEADER	MEDCOM	3	Application dependent information.
Workflow Control Flags	(0029,xx50)	SIEMENS HEADER	MEDCOM	3	Eight free definable flags.
Archive Management Flag Keep Online	(0029,xx51)	SIEMENS HEADER	MEDCOM	3	Flag to control remote archive management system to keep the image always online (also when already archived). Enumerated Values: 00 = remote control not required 01 = keep image online
Archive Management Flag Do Not Archive	(0029,xx52)	SIEMENS HEADER	MEDCOM	3	Flag to control remote archive management system not to archive the related image. Enumerated Values: 00 = remote control not required 01 = don't archive image
Image Location Status	(0029,xx53)	SIEMENS HEADER	MEDCOM	3	Image location status to control retrieving. Defined Terms: ONLINE = retrieving has to be done as usual, NEARLINE = move request to SCP and delay according to value of Estimated Retrieve Time (0029,xx54), OFFLINE = invoking a retrieve operation initiates an operator request, INVALID = invoking a retrieve operation would always result in an error.
Estimated Retrieve Time	(0029,xx54)	SIEMENS HEADER	MEDCOM	3	Estimated retrieve time in seconds. A value less than zero (< 0) indicates location is OFFLINE or INVALID.
Data Size of Retrieved Images	(0029,xx55)	SIEMENS HEADER	MEDCOM	3	Data size of images in MByte.
Siemens Link Sequence	(0029,xx70)	SIEMENS HEADER	MEDCOM	3	Sequence of link items. Each item identify the location of one missing tag. One or more items can be included in this sequence.
Referenced Tag	(0029,xx71)	SIEMENS HEADER	MEDCOM	1	The referenced tag. The value of this tag is in the Child Data Object (CDO). Currently it is always Pixel Data (7FE0,0010).
Referenced Tag Type	(0029,xx72)	SIEMENS HEADER	MEDCOM	1	The Value Representation (type) of the missing tag (e.g. OW). Enumerated values are all DICOM defined Value Representations.
Referenced Value Length	(0029,xx73)	SIEMENS HEADER	MEDCOM	1	The length of the referenced tag value in bytes.
Referenced Object Device Type	(0029,xx74)	SIEMENS HEADER	MEDCOM	1	The Device Type that stores the Child Data Object (CDO) with the referenced tag value. Currently it should be "SHMEM". In future, "SDM", "LOID" or "FILE" are also imaginable. Defined Terms are SHMEM = Shared Memory SDM = Series Data Management LOID = Database FILE
Referenced Object Device Location	(0029,xx75)	SIEMENS HEADER	MEDCOM	2	The Location of the device that stores the Child Data Object (CDO) with the referenced tag value. For the "SHMEM" case, it is the shared memory directory. Can be empty, then the default directory will be taken. In future, for "SDM" this will be the SDM_ID, for FILE it will be the directory name and for "LOID" it will be the database name.
Referenced Object ID	(0029,xx76)	SIEMENS HEADER	MEDCOM	1	The ID of the object that contains the Child Data Object (CDO) with the referenced tag value. In case of "SHMEM" it is the shared memory ID. In future, for "SDM" this will be a Sirius OID, for "FILE" the file name, for "DB"

				the LOID.
Series Work Flow Status	(0029,xx60)	SIEMENS MEDCOM HEADER2	3	syngo Patient Browser specific flags used for clinical work: <ul style="list-style-type: none"> • com = completed • rea = read • ver = verified

8.5.2.1 MEDCOM History Information

The value of the attribute MEDCOM History Information (0029,xx20) is defined in the following way:

Table 63 - MEDCOM History Information

Part	Name	Type	Bytes	Notes
header	Identifier	string	32	Always "CSA HISTORY"
	Version	string	32	e.g. "V1.10"
n Items	Class Name	string	64	
	Modification String	string	1024	

8.5.3 MEDCOM OOG Module

The table in this section contains private IOD Attributes that describe MEDCOM Object Oriented Graphics (OOG). This module is used whenever object graphics is drawn on the image and need to be stored as graphic object properties. Given the condition that the module contents was not removed by other modalities, the graphic objects remain re-animatable if such an image was transferred and is then retrieved back

Table 64 - MEDCOM OOG Module

Attribute Name	Tag	Owner	Type	Notes
MedCom OOG Type	(0029,xx08)	SIEMENS MEDCOM OOG	1	MEDCOM Object Oriented Graphics (OOG) identification characteristics. Defined Terms: MEDCOM OOG 1 MEDCOM OOG 2
MedCom OOG Version	(0029,xx09)	SIEMENS MEDCOM OOG	3	Version of MEDCOM OOG Info (0029,xx10) format.
MedCom OOG Info	(0029,xx10)	SIEMENS MEDCOM OOG	3	MEDCOM Object Oriented Graphics (OOG) data.

The graphics objects are also fully drawn in the Image Overlay Plane for compatibility with other products, which do not support the MedCom OOG module. Any system not supporting the MedCom OOG module shall remove the OOG module and its contents when modifying the image overlay plane content.

8.5.4 syngo Report Data

The module contains private IOD Attributes that describe syngo reports. This module is used when syngo report data are added to DICOM SR and DICOM SC objects.

Table 65 - syngo Report Data

Attribute Name	Tag	Owner	Type	Notes
syngo Report Type	(0029,xx08)	SIEMENS CSA REPORT	1	syngo report characteristics, e.g. report creating application. Defined Terms: CT_LUNGCARE MR_ARGUS This attribute value will be used to identify the corresponding applica-

				tion during generic extension dll management. A restricted character set is used: only A-Z and underscore are supported.
syngo Report Version	(0029,xx09)	SIEMENS CSA REPORT	3	Version of <i>syngo</i> Report Data (0029,xx10) format.
syngo Report Data	(0029,xx10)	SIEMENS CSA ENVELOPE	3	A representation of DICOM SR Attribute Content Sequence (0040,A730). This includes the document relationship and document content. This data will typically be represented using an XML encoding according to a Siemens private scheme.
syngo Report Presentation	(0029,xx11)	SIEMENS CSA ENVELOPE	3	A representation of the recommended presentation for the <i>syngo</i> Report Data (0029,xx10). This presentation will typically be encoded in XSLT.
SR Variant	(0029,xx15)	SIEMENS CSA REPORT		DICOM SR variant. Enumerated Values: 0 = Basic Text SR (1.2.840.10008.5.1.4.1.1.88.11) 1 = Enhanced SR (1.2.840.10008.5.1.4.1.1.88.22) 2 = Comprehensive SR (1.2.840.10008.5.1.4.1.1.88.33) 3 = Mammography CAD SR (1.2.840.10008.5.1.4.1.1.88.50) 4 = Key Object Selection Document (1.2.840.10008.5.1.4.1.1.88.59) 5 = Chest CAD SR (1.2.840.10008.5.1.4.1.1.88.65) 6 = X-Ray Radiation Dose SR (1.2.840.10008.5.1.4.1.1.88.67) 7 = Procedure Log (1.2.840.10008.5.1.4.1.1.88.40)
SC SOP Instance UID	(0029,xx17)	SIEMENS CSA REPORT	3	DICOM SOP Instance UID of <i>syngo</i> based SC Image representing the <i>syngo</i> report object. This UID will be used to identify the Resulting SC object after SR to SC conversion.

8.5.5 syngo Report Info

The module *syngo* Report Info contains all DICOM SR attributes except the Contents Sequence (0040,A730). This module is only used during SR to SC conversion.

8.6 Registry of DICOM Data Elements

Table 66 - Registry of DICOM Data Elements

Tag	Private Owner Code	Name	VR	VM
(0019,xx10)	SIEMENS MR HEADER	MR Header	LO	1
(0029,xx08)	SIEMENS CSA NON-IMAGE	CSA Data Type	CS	1
(0029,xx09)	SIEMENS CSA NON-IMAGE	CSA Data Version	LO	1
(0029,xx10)	SIEMENS CSA NON-IMAGE	CSA Data Info	OB	1
(0029,xx08)	SIEMENS CSA HEADER	CSA Image Header Type	CS	1
(0029,xx09)	SIEMENS CSA HEADER	CSA Image Header Version	LO	1
(0029,xx10)	SIEMENS CSA HEADER	CSA Image Header Info	OB	1
(0029,xx18)	SIEMENS CSA HEADER	CSA Series Header Type	CS	1
(0029,xx19)	SIEMENS CSA HEADER	CSA Series Header Version	LO	1
(0029,xx20)	SIEMENS CSA HEADER	CSA Series Header Info	OB	1

(0029,xx08)	SIEMENS CSA REPORT	syngo Report Type	CS	1
(0029,xx09)	SIEMENS CSA REPORT	syngo Report	LO	1
(0029,xx15)	SIEMENS CSA REPORT	SR Variant	US	1
(0029,xx17)	SIEMENS CSA REPORT	SC SOP Instance UID	UI	1
(0029,xx10)	SIEMENS CSA ENVELOPE	syngo Report Data	OB	1
(0029,xx11)	SIEMENS CSA ENVELOPE	syngo Report Presentation	OB	1
(0029,xx08)	SIEMENS MEDCOM HEADER	MedCom Header Type	CS	1
(0029,xx09)	SIEMENS MEDCOM HEADER	MedCom Header Version	LO	1
(0029,xx10)	SIEMENS MEDCOM HEADER	MedCom Header Info	OB	1
(0029,xx20)	SIEMENS MEDCOM HEADER	MedCom History Information	OB	1
(0029,xx40)	SIEMENS MEDCOM HEADER	Application Header Sequence	SQ	1
(0029,xx41)	SIEMENS MEDCOM HEADER	Application Header Type	CS	1
(0029,xx42)	SIEMENS MEDCOM HEADER	Application Header ID	LO	1
(0029,xx43)	SIEMENS MEDCOM HEADER	Application Header Version	LO	1
(0029,xx44)	SIEMENS MEDCOM HEADER	Application Header Info	OB	1
(0029,xx50)	SIEMENS MEDCOM HEADER	Workflow Control Flags	LO	8
(0029,xx51)	SIEMENS MEDCOM HEADER	Arch. Management Flag Keep Online	CS	1
(0029,xx52)	SIEMENS MEDCOM HEADER	Arch. Mgmt Flag Do Not Archive	CS	1
(0029,xx53)	SIEMENS MEDCOM HEADER	Image Location Status	CS	1
(0029,xx54)	SIEMENS MEDCOM HEADER	Estimated Retrieve Time	DS	1
(0029,xx55)	SIEMENS MEDCOM HEADER	Data Size of Retrieved Images	DS	1
(0029,xx70)	SIEMENS MEDCOM HEADER	Siemens Link Sequence	SQ	1
(0029,xx71)	SIEMENS MEDCOM HEADER	Referenced Tag	AT	1
(0029,xx72)	SIEMENS MEDCOM HEADER	Referenced Tag Type	CS	1
(0029,xx73)	SIEMENS MEDCOM HEADER	Referenced Value Length	UL	1
(0029,xx74)	SIEMENS MEDCOM HEADER	Referenced Object Device Type	CS	1
(0029,xx75)	SIEMENS MEDCOM HEADER	Referenced Object Device Location	OB	1
(0029,xx76)	SIEMENS MEDCOM HEADER	Referenced Object ID	OB	1
(0029,xx60)	SIEMENS MEDCOM HEADER2	Series Work Flow Status	LO	1
(0029,xx08)	SIEMENS MEDCOM OOG	MedCom OOG Type	CS	1
(0029,xx09)	SIEMENS MEDCOM OOG	MedCom OOG Version	LO	1
(0029,xx10)	SIEMENS MEDCOM OOG	MedCom OOG Info	OB	1
(7FE1,xx10)	SIEMENS CSA NON-IMAGE	CSA Data	OB	1

8.7 Standard Extension of all SOP Classes

Table 67 - data dictionary of all DICOM IOD attributes where the DICOM standard definitions are extended:

Attribute Name	Tag	Private Creator	Type	Notes
Image Type	(0008,0008)	-	1	see A.4.1 additional Defined Terms: Defined Terms for value 3: OTHER Defined Terms for value 4: CSA 3D EDITOR CSA 3D FLY PATH CSA 3D FLY VRT CSA 3D FUSION CSA AVERAGE CSA BLACK IMAGE CSA RESAMPLED CSA MIP CSA MPR

				CSA MPR CURVED CSA MPR THICK CSA SSD CSA SUBTRACT CT_SOM4 * SHS *
Patient Position	(0018,5100)	-	2C	see A.4.2 additional Defined Terms for the Magnetom Open: HLS HLP FLS FLP HLDL HLDR FLDL FLDR

All SOP classes may contain additional type 3 attributes which DICOM standard defines in a different DICOM IOD or DICOM SOP class (attributes from Normalized SOP classes).

This is the case for example for

- Rescale Slope (0028,1053)
 - Rescale Intercept (0028,1052)
- which are also used in the MR IOD.

8.7.1 Image Type

The Image Type (0008,0008) attribute identifies important image identification characteristics. These characteristics are:

1. Pixel Data Characteristics:

- is the image an ORIGINAL Image; an image whose pixel values are based on original or source data, or
- is the image a DERIVED Image; an image whose pixel values have been derived in some manner from the pixel value of one or more other images.

2. Patient Examination Characteristics:

- is the image a PRIMARY Image; an image created as a direct result of the Patient examination, or
- is the image a SECONDARY Image; an image created after the initial Patient examination.

3. Modality Specific Characteristics (SOP Specific Characteristics).

4. Implementation specific identifiers; other implementation specific identifiers shall be documented in an implementation's conformance claim.

The Image Type attribute is multi-valued and shall be provided in the following manner:

- Value 1 shall identify the Pixel Data Characteristics; Enumerated Values for the Pixel Data Characteristics are:
 - ORIGINAL = identifies an Original Image
 - DERIVED = identifies a Derived Image

- Value 2 shall identify the Patient Examination Characteristics; Enumerated Values for the Patient Examination Characteristics are:
 - PRIMARY = identifies a Primary Image
 - SECONDARY = identifies a Secondary Image
- Value 3 shall identify any Image IOD specific specialization, the following terms are defined in addition to the DICOM standard definitions:
 - OTHER = is also used for converted non-Axial and non-Localizer CT images
 - MPR = for 3D MPR images
 - PROJECTION IMAGE = for 3D MIP and SSD images
- Value 4 which are implementation specific, the following terms are defined in addition to the DICOM standard definitions:
 - original *syngo* generated data set types:
 - CSA 3D EDITOR = object created by 3D Editor
 - CSA 3D FLY PATH = object created by Fly Through Path
 - CSA 3D FLY VRT = object created by Fly Through Volume Rendering Technique
 - CSA 3D FUSION = object created by Fusion
 - CSA AVERAGE = image was created by Average
 - CSA BLACK IMAGE = SC Image with black pixels, only graphics information is of interest
 - CSA RESAMPLED = derived image created by zooming or panning original image
 - CSA REPORT = *syngo* reporting (documentation of diagnosis)
 - CSA RESULT = *syngo* reporting (postprocessing results)
 - CSA MIP = image created by Maximum Intensity Projection
 - CSA MIP THIN = image created by Maximum Intensity Projection
 - CSA MPR = image created by Multi Planar Reconstruction
 - CSA MPR CURVED = image created by Multi Planar Reconstruction
 - CSA MPR THICK = image created by Multi Planar Reconstruction
 - CSA MPR THIN = image created by Multi Planar Reconstruction
 - CSA SSD = SC Image as Shaded Surface Display
 - CSA SUBTRACT = image was created by Subtraction
 - Converted images
 - CT_SOM4 NONE = converted SOMARIS image
 - CT_SOM4 CONV = converted SOMARIS Convolution Kernel file
 - CT_SOM4 DART = converted SOMARIS Dental Artificial image
 - CT_SOM4 DEVA = converted SOMARIS Dental Evaluation image
 - CT_SOM4 DGRA = converted SOMARIS Dental Graphics image
 - CT_SOM4 DMEA = converted SOMARIS Dynamic Measurement image
 - CT_SOM4 DPAN = converted SOMARIS Dental Panorama image
 - CT_SOM4 DPAR = converted SOMARIS Dental Paraxial image
 - CT_SOM4 EBT = converted SOMARIS Evolution image
 - CT_SOM4 HIS = converted SOMARIS Histogram Graphics image
 - CT_SOM4 HISC = converted SOMARIS Histogram Graphics image
 - CT_SOM4 MUL = converted SOMARIS Multiscan image
 - CT_SOM4 OEVA = converted SOMARIS Osteo Evaluation image
 - CT_SOM4 OTOM = converted SOMARIS Osteo Tomogram image
 - CT_SOM4 OTOP = converted SOMARIS Osteo Topogram image
 - CT_SOM4 PLOT = converted SOMARIS Plot image
 - CT_SOM4 QUAL = converted SOMARIS Quality image
 - CT_SOM4 R2D = converted SOMARIS 2D Rebuild image
 - CT_SOM4 R3D = converted SOMARIS 3D Rebuild image
 - CT_SOM4 R3DE = converted SOMARIS 3D Rebuild image

CT_SOM4 RMAX = converted SOMARIS Maximum Intensity Projection image
 CT_SOM4 RMIN = converted SOMARIS Minimum Intensity Projection image
 CT_SOM4 ROT = converted SOMARIS Rotation Mode image
 CT_SOM4 RRAD = converted SOMARIS Radiographic Projection image
 CT_SOM4 RVIT = converted SOMARIS Vessel Image Tool image
 CT_SOM4 RVRT = converted SOMARIS Volumetric Rendering image
 CT_SOM4 SAVE = converted SOMARIS Evolution Screen Save image
 CT_SOM4 SCAN = converted SOMARIS Standard Mode image
 CT_SOM4 SEQ = converted SOMARIS Sequence Mode image
 CT_SOM4 SER = converted SOMARIS Serial Mode image
 CT_SOM4 SIN = converted SOMARIS Sinogram image
 CT_SOM4 SINC = converted SOMARIS Sinogram image
 CT_SOM4 SPI = converted SOMARIS Spiral Mode image
 CT_SOM4 STA = converted SOMARIS Static Mode image
 CT_SOM4 TAB = converted SOMARIS Correction Table image
 CT_SOM4 TOP = converted SOMARIS Topogram image
 CT_SOM4 GTOP = converted SOMARIS Topo Graphics image
 CT_SOM4 PEVG = converted SOMARIS Pulmo Evaluation image
 CT_SOM4 PEVI = converted SOMARIS Pulmo Evaluation image
 CT_SOM4 PUL = converted SOMARIS Pulmo Respiration image
 CT_SOM4 PROT = converted SOMARIS Protocol image
 CT_SOM4 TEXT = converted SOMARIS Text image
 CT_SOM4 ICD = converted SOMARIS Interventional Cine image
 SHS DENT = converted MagicView Dental Tomogram image
 SHS DPAN = converted MagicView Dental Panorama image
 SHS DPAR = converted MagicView Dental Paraxial image
 SHS 3D_CURVED = converted MagicView image
 SHS 3D_MIP = converted MagicView Maximum Intensity Projection image
 SHS 3D_MPR = converted MagicView Multi Planar Reconstruction image
 SHS 3D_SSD = converted MagicView Shaded Surface Display image
 SHS 3D_VRT = converted MagicView Volumetric Rendering image

8.7.1.1 MR Image Type

For MR Image Objects starting from value 3 the following terms are defined in addition to the DICOM standard definitions. The image type values are specified as defined terms and the nature is application specific. There is no guarantee for completeness and interoperability.

Online Reconstruction:

R	Real Part Image
M	Magnitude Image
P	Phase Image

Normalize and Distortion Correction

NORM	Normalized Pixel
ND	Not distorted Pixel
DIS2D	Distorted Pixel and remapped

Diffusion:

ADC	Apparent Diffusion Coefficient
-----	--------------------------------

Stroke Perfusion:

TTP	Time To Peak
PBP	Percent-of-Baseline at Peak
GBP	Global Average Bolus Curve Plotted
RELCBV	Relative Cerebral Blood Volume

RELCBF	Relative Cerebral Blood Flow
RELMTT	Relative Mean Transit Time
Breast Perfusion	
TTP	Time To Peak
WI	Wash In
WO	Wash Out
PEI	Positive Enhancement Integral
MITP	Maximum Intensity Time Projection
COMB	Combination
Phase Contrast Angio	
MAG	Magnitude Images
MSUM	Magnitude Sum Image
fMRI:	
MEAN	Mean Value Image
TTEST	Student's t-test (for each slice over the repetitions)
MOSAIC	Square Mosaic Image (N x N) N=Slice
COR	Correlation (for each slice over the repetitions)
RETRO	Retro Image
DUMMY IMAGE	Dummy Image
Filter	
MOCO	Motion Correction
FILTERED	Motion Correction Filter (product type specific)
IMAGEFILTER	Image Filter
Subtraction	
SUB	Subtraction
Inline-Processing:	
MIP_SAG	Online Maximum Intensity Projections sagital
MIP_COR	Online Maximum Intensity Projections coronal
MIP_TRA	Online Maximum Intensity Projections transversal
TMIP	Online Temporal Maximum Intensity Projections
TMIP_SAG	Online Temporal Maximum Intensity Projections sagital
TMIP_COR	Online Temporal Maximum Intensity Projections coronal
TMIP_TRA	Online Temporal Maximum Intensity Projections transversal
TSTDDEV	Online Standard Deviation temporal
STDDEV_SAG	Online Standard Deviation temporal sagital
STDDEV_COR	Online Standard Deviation temporal coronal
STDDEV_TRA	Online Standard Deviation temporal transversal
NORM	Normalize Algorithm
ND	Not Distortion Corrected
DIS2D	Distortion Correction 2D
DIS3D	Distortion Correction 3D
RETRO	Retrospective Gating
MOCO	Motion Correction (Motion Detection and Interpolation)
FILTERED	Online Post-processing Filter
FIL	Inline Image Filter
PROJECTION IMAGE	Projection Image
Dynamic Analysis	
ADD	Addition
MEAN	Arithmetic Mean

COR	Correlation
DIFFER	Differentiation
DIFFUS	Diffusion Coefficient
DIV	Division
INT	Integration
LOG	Logarithm
MULT	Multiplication
SLOPE	Slope
SDEV	Standard Deviation
SUB	Subtraction
T1	Longitudinal Relaxation Time
PDT1	T1 Weighted Proton Density
T2	Transversal Relaxation Time
PDT2	T2 Weighted Proton Density
TTP	Time To Peak
TTEST	Difference between the mean values of the group A and group B in units of the corresponding combined standard deviation
CVxx	Context Vision Filter, xx defines grade of the filter

Spectroscopy

SPEC	MR-Object, Spectral Map or Metabolite Image
------	---

Graphical Slice Positioning

GSP	Graphical Slice Positioning
-----	-----------------------------

Position Display

POSDISP	Position Display
---------	------------------

Mean Curve

CSA BLACK IMAGE	Diagram and Result Table(s)
-----------------	-----------------------------

Image Composing

COMPOSED	Composed Images
----------	-----------------

- DIXON Images

FAT_FRACTION	Fat Fraction
R2_STAR_MAP	R2 Star Map
WATER	Water
FAT	Fat
IN_PHASE	In Phase
OUT_PHASE	Out Phase
FIELD_MAP	Field Map
WATER_FRACTION	Water Fraction

8.8 DICOM Print SCU – detailed status displays

The following tables document the behavior of the <product> DICOM Print AE in response to messages received for the printer SOP class and the print job SOP class.

Definitions of camera symbols:

- Idle: Camera is installed and ready; idle icon is displayed.

- **Interact:** The user has to react in near future, but not immediately.
Example: A camera was low in 8x10 clear sheets: LOW 8x10 CLR was sent by n-event-report.
- **Queue Stopped:** The user has to react immediately. Either the camera needs immediate interaction or a job has been aborted.
Example: A camera is out of 8x10 clear sheets, or camera is down, or a film job is aborted.

Note: different camera symbols are displayed according to the Printer Status Info.

8.8.1 Common Status Information

Table 68 - "Common Status Info evaluation"

Printer Status Info/ Execution Status Info	Description	Message string visible in 'Status Bar'	Other action for UI/ 'camera symbol'
NORMAL	Camera is ready	Camera is ready	<None>/idle
BAD RECEIVE MGZ	There is a problem with the film receive magazine. Films from the printer cannot be transported into the magazine.	Problem with receive magazine.	<None>/interact
BAD SUPPLY MGZ	There is a problem with the film supply magazine. Films from this magazine cannot be transported into the printer.	Problem with supply magazine.	<None>/interact
CALIBRATING	Printer is performing self calibration, it is expected to be available for normal operation shortly.	Self calibration. Please wait.	<None>/idle
CALIBRATION ERR	An error in the printer calibration has been detected, quality of processed films may not be optimal.	Problem in calibration. Film quality may not be optimal.	<None>/interact
CHECK CHEMISTRY	A problem with the processor chemicals has been detected, quality of processed films may not be optimal.	Problem with chemistry. Film quality may not be optimal.	<None>/interact
CHECK SORTER	There is an error in the film sorter	Error in film sorter.	<None>/interact
CHEMICALS EMPTY	There are no processing chemicals in the processor, films will not be printed and processed until the processor is back to normal.	Camera chemistry empty. Please check.	<None>/interact
CHEMICALS LOW	The chemical level in the processor is low, if not corrected, it will probably shut down soon.	Camera chemistry low. Please check.	<None>/interact
COVER OPEN	One or more printer or processor covers, drawers, doors are open.	Camera cover, drawer or door open.	<None>/interact
ELEC CONFIG ERR	Printer configured improperly for this job.	Camera configured improperly for this job. Queue stopped.	Queue for this camera will be STOPPED/ Queue stopped
ELEC DOWN	Printer is not operating due to some unspecified electrical hardware problem.	Camera electrical hardware Problem.	<None>/interact
ELEC SW ERROR	Printer not operating for some unspecified software error.	Camera software problem. Queue stopped.	Queue for this camera will be STOPPED/ Queue stopped
EMPTY 8X10	The 8x10 inch film supply magazine is empty.	8x10 film supply empty.	<None>/interact
EMPTY 8X10 BLUE	The 8x10 inch blue film supply magazine is empty.	8x10 blue film supply empty.	<None>/interact
EMPTY 8X10 CLR	The 8x10 inch clear film supply magazine is empty.	8x10 clear film supply empty.	<None>/interact
EMPTY 8X10 PAPR	The 8x10 inch paper supply magazine is empty.	8x10 paper supply empty.	<None>/interact
EMPTY 10X12	The 10x12 inch film supply magazine is empty.	10x12 film supply empty.	<None>/interact
EMPTY 10X12 BLUE	The 10x12 inch blue film supply magazine is empty.	10x12 blue film supply empty.	<None>/interact
EMPTY 10X12 CLR	The 10x12 inch clear film supply magazine is empty.	10x12 clear film supply empty.	<None>/interact
EMPTY 10X12 PAPR	The 10x12 inch paper supply magazine is empty.	10x12 paper supply empty.	<None>/interact

Printer Status Info/ Execution Status Info	Description	Message string visible in 'Status Bar'	Other action for UI/ 'camera symbol'
EMPTY 10X14	The 10x14 inch film supply magazine is empty.	10x14 film supply empty.	<None>/interact
EMPTY 10X14 BLUE	The 10x14 inch blue film supply magazine is empty.	10x14 blue film supply empty.	<None>/interact
EMPTY 10X14 CLR	The 10x14 inch clear film supply magazine is empty.	10x14 clear film supply empty.	<None>/interact
EMPTY 10X14 PAPER	The 10x14 inch paper supply magazine is empty.	10x14 paper supply empty.	<None>/interact
EMPTY 11X14	The 11x14 inch film supply magazine is empty.	11x14 film supply empty.	<None>/interact
EMPTY 11X14 BLUE	The 11x14 inch blue film supply magazine is empty.	11x14 blue film supply empty.	<None>/interact
EMPTY 11X14 CLR	The 11x14 inch clear film supply magazine is empty.	11x14 clear film supply empty.	<None>/interact
EMPTY 11X14 PAPER	The 11x14 inch paper supply magazine is empty.	11x14 paper supply empty.	<None>/interact
EMPTY 14X14	The 14x14 inch film supply magazine is empty.	14x14 film supply empty.	<None>/interact
EMPTY 14X14 BLUE	The 14x14 inch blue film supply magazine is empty.	14x14 blue film supply empty.	<None>/interact
EMPTY 14X14 CLR	The 14x14 inch clear film supply magazine is empty.	14x14 clear film supply empty.	<None>/interact
EMPTY 14X14 PAPER	The 14x14 inch paper supply magazine is empty.	14x14 paper supply empty.	<None>/interact
EMPTY 14X17	The 14x17 inch film supply magazine is empty.	14x17 film supply empty.	<None>/interact
EMPTY 14X17 BLUE	The 14x17 inch blue film supply magazine is empty.	14x17 blue film supply empty.	<None>/interact
EMPTY 14X17 CLR	The 14x17 inch clear film supply magazine is empty.	14x17 clear film supply empty.	<None>/interact
EMPTY 14X17 PAPER	The 14x17 inch paper supply magazine is empty.	14x17 paper supply empty.	<None>/interact
EMPTY 24X24	The 24x24 inch film supply magazine is empty.	24x24 film supply empty.	<None>/interact
EMPTY 24X24 BLUE	The 24x24 inch blue film supply magazine is empty.	24x24 blue film supply empty.	<None>/interact
EMPTY 24X24 CLR	The 24x24 inch clear film supply magazine is empty.	24x24 clear film supply empty.	<None>/interact
EMPTY 24X24 PAPER	The 24x24 inch paper supply magazine is empty.	24x24 paper supply empty.	<None>/interact
EMPTY 24X30	The 24x30 inch film supply magazine is empty.	24x30 film supply empty.	<None>/interact
EMPTY 24X30 BLUE	The 24x30 inch blue film supply magazine is empty.	24x30 blue film supply empty.	<None>/interact
EMPTY 24X30 CLR	The 24x30 inch clear film supply magazine is empty.	24x30 clear film supply empty.	<None>/interact
EMPTY 24X30 PAPER	The 24x30 inch paper supply magazine is empty.	24x30 paper supply empty.	<None>/interact
EMPTY A4 PAPER	The A4 paper supply magazine is empty.	A4 paper supply empty.	<None>/interact
EMPTY A4 TRANS	The A4 transparency supply magazine is empty.	A4 transparency supply empty.	<None>/interact
EXPOSURE FAILURE	The exposure device has failed due to some unspecified reason.	Exposure device has failed.	<None>/interact
FILM JAM	A film transport error has occurred and a film is jammed in the printer or processor.	Film jam.	<None>/interact
FILM TRANSP ERR	There is a malfunction with the film transport, there may or may not be a film jam.	Film transport problem.	<None>/interact
FINISHER EMPTY	The finisher is empty.	Finisher is empty.	<None>/interact
FINISHER ERROR	The finisher is not operating due to some unspecified reason.	Finisher problem.	<None>/interact
FINISHER LOW	The finisher is low on supplies.	Finisher low.	<None>/interact
LOW 8X10	The 8x10 inch film supply magazine is low.	8x10 film supply low.	<None>/interact
LOW 8X10 BLUE	The 8x10 inch blue film supply magazine is low.	8x10 blue film supply low.	<None>/interact

Printer Status Info/ Execution Status Info	Description	Message string visible in 'Status Bar'	Other action for UI/ 'camera symbol'
LOW 8X10 CLR	The 8x10 inch clear film supply magazine is low.	8x10 clear film supply low.	<None>/interact
LOW 8X10 PAPR	The 8x10 inch paper supply magazine is low.	8x10 paper supply low.	<None>/interact
LOW 10X12	The 10x12 inch film supply magazine is low.	10x12 film supply low.	<None>/interact
LOW 10X12 BLUE	The 10x12 inch blue film supply magazine is low.	10x12 blue film supply low.	<None>/interact
LOW 10X12 CLR	The 10x12 inch clear film supply magazine is low.	10x12 clear film supply low.	<None>/interact
LOW 10X12 PAPR	The 10x12 inch paper supply magazine is low.	10x12 paper supply low.	<None>/interact
LOW 10X14	The 10x14 inch film supply magazine is low.	10x14 film supply low.	<None>/interact
LOW 10X14 BLUE	The 10x14 inch blue film supply magazine is low.	10x14 blue film supply low.	<None>/interact
LOW 10X14 CLR	The 10x14 inch clear film supply magazine is low.	10x14 clear film supply low.	<None>/interact
LOW 10X14 PAPR	The 10x14 inch paper supply magazine is low.	10x14 paper supply low.	<None>/interact
LOW 11X14	The 11x14 inch film supply magazine is low.	11x14 film supply low.	<None>/interact
LOW 11X14 BLUE	The 11x14 inch blue film supply magazine is low.	11x14 blue film supply low.	<None>/interact
LOW 11X14 CLR	The 11x14 inch clear film supply magazine is low.	11x14 clear film supply low.	<None>/interact
LOW 11X14 PAPR	The 11x14 inch paper supply magazine is low.	11x14 paper supply low.	<None>/interact
LOW 14X14	The 14x14 inch film supply magazine is low.	14x14 film supply low.	<None>/interact
LOW 14X14 BLUE	The 14x14 inch blue film supply magazine is low.	14x14 blue film supply low.	<None>/interact
LOW 14X14 CLR	The 14x14 inch clear film supply magazine is low.	14x14 clear film supply low.	<None>/interact
LOW 14X14 PAPR	The 14x14 inch paper supply magazine is low.	14x14 paper supply low.	<None>/interact
LOW 14X17	The 14x17 inch film supply magazine is low.	14x17 film supply low.	<None>/interact
LOW 14X17 BLUE	The 14x17 inch blue film supply magazine is low.	14x17 blue film supply low.	<None>/interact
LOW 14X17 CLR	The 14x17 inch clear film supply magazine is low.	14x17 clear film supply low.	<None>/interact
LOW 14X17 PAPR	The 14x17 inch paper supply magazine is low.	14x17 paper supply low.	<None>/interact
LOW 24X24	The 24x24 inch film supply magazine is low.	24x24 film supply low.	<None>/interact
LOW 24X24 BLUE	The 24x24 inch blue film supply magazine is low.	24x24 blue film supply low.	<None>/interact
LOW 24X24 CLR	The 24x24 inch clear film supply magazine is low.	24x24 clear film supply low.	<None>/interact
LOW 24X24 PAPR	The 24x24 inch paper supply magazine is low.	24x24 paper supply low.	<None>/interact
LOW 24X30	The 24x30 inch film supply magazine is low.	24x30 film supply low.	<None>/interact
LOW 24X30 BLUE	The 24x30 inch blue film supply magazine is low.	24x30 blue film supply low.	<None>/interact
LOW 24X30 CLR	The 24x30 inch clear film supply magazine is low.	24x30 clear film supply low.	<None>/interact
LOW 24X30 PAPR	The 24x30 inch paper supply magazine is low.	24x30 paper supply low.	<None>/interact
LOW A4 PAPR	The A4 paper supply magazine is low.	A4 paper supply low.	<None>/interact
LOW A4 TRANS	The A4 transparency supply magazine is low.	A4 transparency supply low.	<None>/interact
NO RECEIVE MGZ	The film receive magazine is not available.	Film receiver not available.	<None>/interact
NO RIBBON	The ribbon cartridge needs to be replaced.	Replace ribbon cartridge.	<None>/interact
NO SUPPLY MGZ	The film supply magazine is not available.	Film supply not available.	<None>/interact

Printer Status Info/ Execution Status Info	Description	Message string visible in 'Status Bar'	Other action for UI/ 'camera symbol'
CHECK PRINTER	The printer is not ready at this time, operator intervention is required to make the printer available.	Check camera.	<None>/interact
CHECK PROC	The processor is not ready at this time, operator intervention is required to make the printer available.	Check processor.	<None>/interact
PRINTER DOWN	The printer is not operating due to some unspecified reason.	Camera down.	<None>/interact
PRINTER INIT	The printer is not ready at this time, it is expected to become available without intervention. For example, it may be in a normal warm-up state.	Camera initializing.	<None>/Idle
PRINTER OFFLINE	The printer has been disabled by an operator or service person.	Camera off-line.	<None>/interact
PROC DOWN	The processor is not operating due to some unspecified reason.	Processor down.	<None>/interact
PROC INIT	The processor is not ready at this time, it is expected to become available without intervention. For example, it may be in a normal warm-up state.	Processor initializing.	<None>/Idle
PROC OVERFLOW FL	Processor chemicals are approaching the overflow full mark.	Processor chemicals near overflow.	<None>/interact
PROC OVERFLOW HI	Processor chemicals have reached the overflow full mark.	Processor chemicals overflow.	<None>/interact
QUEUED	Print job in Queue	--	<None>/Idle
RECEIVER FULL	The film receive magazine is full.	Receiver full.	<None>/interact
REQ MED NOT INST	The requested film, paper, or other media supply magazine is installed in the printer, but may be available with operator intervention.	Install media supply.	<None>/interact
REQ MED NOT AVAI	The requested film, paper, or other media requested is not available on this printer.	Media supply not available on this camera. Queue stopped. Change camera.	Queue for this camera will be STOPPED/ Queue stopped
RIBBON ERROR	There is an unspecified problem with the print ribbon.	Error with print ribbon.	<None>/interact
SUPPLY EMPTY	The printer is out of film.	Camera out of film.	<None>/interact
SUPPLY LOW	The film supply is low.	Film supply low.	<None>/interact
UNKNOWN	There is an unspecified problem.	Unspecified problem with camera.	<None>/interact

8.8.2 Additional Status Information – AGFA printers

Table 69 - "Additional Agfa printer Status Info evaluation"

Printer Status Info/ Execution Status Info	Description	Message string visible in 'Status Bar'	Other action for UI/ 'camera symbol'
WARMING UP	Printer is in the warm-up stage. Spooling of print jobs to disk is still possible.	Camera is warming up.	<None>/idle
OFFLINE	OFFLINE Printer is switched off-line. Spooling of print jobs to disk is still possible.	Camera is switched off-line.	<None>/interact
NONE	General printer warning, no specific information is available. Spooling of print jobs to disk is still possible.	--	<None>/idle

8.8.3 Additional Status Information – Kodak PACS Link (formerly Imation)

Table 70 - "Additional Kodak PACS Link (Imation) printer Status Info evaluation"

Printer Status Info/ Execution Status Info	Description	Message string visible in 'Status Bar'	Other action for UI/ 'camera symbol'
---	-------------	---	---

Printer Status Info/ Execution Status Info	Description	Message string visible in 'Status Bar'	Other action for UI/ 'camera symbol'
SUPPLY MGZ ERR	The supply magazine has an error.	Film supply has an error.	<None>/interact

8.8.4 Additional Status Information – Kodak 1901

Table 71 - "Additional Kodak 190 printer Status Info evaluation"

Printer Status Info/ Execution Status Info	Description	Message string visible in 'Status Bar'	Other action for UI/ 'camera symbol'
PRINTER STOPPED	The printer has stopped.	Camera has stopped.	<None>/interact
FATAL ERROR	Fatal Error.	Fatal Error. Queue stopped.	Queue for this camera will be STOPPED/ Queue stopped

8.8.5 Additional Status Information – Kodak 2180/1120

Table 72 - "Additional Kodak 2180/1120 printer Status Info evaluation"

Printer Status Info/ Execution Status Info	Description	Message string visible in 'Status Bar'	Other action for UI/ 'camera symbol'
PRINTER NOT RDY	Printer not ready.	Camera not ready.	<None>/interact
CHECK PROCESSOR	Check processor.	Check processor.	<None>/interact
NO TONER	No toner.	No toner.	<None>/interact
FATAL	Fatal Error.	Fatal Error. Queue stopped.	Queue for this camera will be STOPPED/ Queue stopped

8.8.6 Additional Status Information – Codonics

Table 73 - "Additional Codonics printer Status Info evaluation"

Printer Status Info/ Execution Status Info	Description	Message string visible in 'Status Bar'	Other action for UI/ 'camera symbol'
STANDARD	Printer is ready.	Camera is ready.	<None>/Normal
LOAD A-SIZE	Load A-Size media.	Load A-Size media.	<None>/interact
LOAD A-DVPAPER	Load A-Size black and white paper.	Load A-Size black and white paper.	<None>/interact
LOAD A-CVPAPER	Load A-Size color paper.	Load A-Size color paper.	<None>/interact
LOAD A-CVTRANS	Load A-Size transparencies.	Load A-Size transparen- cies.	<None>/interact
LOAD A4-SIZE	Load A4-Size media.	Load A4-Size media.	<None>/interact
LOAD A4-DVPAPER	Load A4-Size black and white paper.	Load A4-Size black and white paper.	<None>/interact
LOAD A4-CVPAPER	Load A4-Size color paper.	Load A4-Size color pa- per.	<None>/interact
LOAD A4-CVTRANS	Load A4-Size transparencies.	Load A4-Size transpar- encies.	<None>/interact
LOAD LA-SIZE	Load LA-Size media.	Load LA-Size media.	<None>/interact
LOAD LA-DVPAPER	Load LA-Size black and white paper.	Load LA-Size black and white paper.	<None>/interact
LOAD LA-CVPAPER	Load LA-Size color paper.	Load LA-Size color pa- per.	<None>/interact
LOAD LA-CVTRANS	Load LA-Size transparencies.	Load LA-Size transpar- encies.	<None>/interact
LOAD LA4-SIZE	Load LA4-Size media.	Load LA4-Size media.	<None>/interact
LOAD LA4-DVPAPER	Load LA4-Size black and white paper.	Load LA4-Size black and white paper.	<None>/interact
LOAD LA4-CVPAPER	Load LA4-Size color paper.	Load LA4-Size color paper.	<None>/interact

Printer Status Info/ Execution Status Info	Description	Message string visible in 'Status Bar'	Other action for UI/ 'camera symbol'
LOAD LA4-CVTRANS	Load LA4-Size transparencies.	Load LA4-Size transparencies.	<None>/interact
LOAD XLA-SIZE	Load XLA-Size media.	Load XLA-Size media.	<None>/interact
LOAD XLA-DVPAPER	Load XLA-Size black and white paper.	Load XLA-Size black and white paper.	<None>/interact
LOAD XLA-CVPAPER	Load XLA-Size color paper.	Load XLA-Size color paper.	<None>/interact
LOAD XLA-CVTRANS	Load XLA-Size transparencies.	Load XLA-Size transparencies.	<None>/interact
LOAD XLA4-SIZE	Load XLA4-Size media.	Load XLA4-Size media.	<None>/interact
LOAD XLA4-DVPAPER	Load XLA4-Size black and white paper.	Load XLA4-Size black and white paper.	<None>/interact
LOAD XLA4-CVPAPER	Load XLA4-Size color paper.	Load XLA4-Size color paper.	<None>/interact
LOAD XLA4-CVTRANS	Load XLA4-Size transparencies.	Load XLA4-Size transparencies.	<None>/interact
LOAD XLW-SIZE	Load XLW-Size media.	Load XLW-Size media.	<None>/interact
LOAD XLW-DVPAPER	Load XLW-Size black and white paper.	Load XLW-Size black and white paper.	<None>/interact
LOAD XLW-CVPAPER	Load XLW-Size color paper.	Load XLW-Size color paper.	<None>/interact
LOAD 8X10-SIZE	Load 8x10 media.	Load 8x10 media.	<None>/interact
LOAD 8X10-DVFILM	Load XLW-Size black and white film.	Load XLW-Size black and white film.	<None>/interact
SUPPLY MISSING	The film supply magazine specified for this job is not available.	Film supply not available.	<None>/interact
RIBBON MISSING	Ribbon is missing.	Ribbon is missing.	<None>/interact
RIBBON EMPTY	Ribbon is empty.	Ribbon is empty.	<None>/interact
TOP COVER OPEN	Top cover of printer is open.	Top cover of camera is open.	<None>/interact

8.8.7 Additional DICOM Execution Status Information Evaluation

Table 74 - "Additional DICOM Execution Status Info evaluation"

Printer Status Info/ Execution Status Info	Description	Message string visible in 'Status Bar'	Other action for UI/ 'camera symbol'
INVALID PAGE DES	The specified page layout cannot be printed or other page description errors have been detected.	Film Job cannot be printed on this camera. Queue stopped. Please redirect film job.	Queue for this camera will be STOPPED/ Queue stopped
INSUFFICIENT MEMORY	There is not enough memory available to complete this job.	Not enough memory available in camera. Queue stopped. Please continue queue or change camera.	Queue for this camera will be STOPPED/ Queue stopped
NONE	General printer warning, no specific information is available. Spooling of print jobs to disk is still possible.	--	<None>/Idle

8.8.8 Additional DICOM Execution Status Information

Printer Status Info and Execution Status Info are defined terms and can therefore be extended or reduced by camera manufacturers. Therefore syngo shall be flexible.

If any other printer status info or execution status info is received, syngo will react as shown in the following table:

Table 75 - Additional DICOM Execution Status Information

Printer Status / Execution	Printer / Execution Status Info	Description	Message string visible in the HCD status bar	Other action for syngo / camera symbol
----------------------------	---------------------------------	-------------	--	--

Printer Status / Execution	Printer / Execution Status Info	Description	Message string visible in the HCD status bar	Other action for syngo / camera symbol
WARNING	<any other>	<not defined status info>	Camera info: <status info>	<None>/Interact
FAILURE	<any other>	<not defined status info>	Camera info: <status info> Queue stopped.	Queue for this camera will be STOPPED/ Queue stopped

Annex A: Index of Tables

Table 1 - Network Services	2
Table 2 - Media Services.....	4
Table 3 - Implementation Identifying Information	4
Table 4 - Presentation Context Table "Verification"	17
Table 5 - Presentation Context Table "Send to ...".	20
Table 6 - Presentation Context Table "Update Flag Information"	23
Table 7 - Presentation Context Table "Return Commitment Result"	25
Table 8 - Status codes "Save to local disk"	25
Table 9 - Presentation Context Table "Save to local disk"	27
Table 10 - Order of Preference Transfer Syntax	28
Table 11 - Presentation Context Table "Evaluate Commit Request"	31
Table 12 - Supported DIMSE-C Operations - Query/Retrieve SCU	33
Table 13 - Presentation Context Table "Search..."	34
Table 14 - C-FIND RQ Search Keys	35
Table 15 - Status Codes "Search..."	37
Table 16 - Presentation Context Table "Import..."	37
Table 17 - C-MOVE RSP Status Codes	38
Table 18 - Presentation Context Table "Process Search Requests"	40
Table 19 - Query/Retrieve SCP supported attributes.....	41
Table 20 - Status Codes Process Search Request.....	44
Table 21 - Presentation Context Table "Process Retrieve Requests"	44
Table 22 - Status Codes "Process Retrieve Requests"	45
Table 23 - Presentation Context Table "Print Film"	47
Table 24 - Basic Film Session N-CREATE attributes	48
Table 25 - Basic Film Session Status Codes	48
Table 26 - Basic Film Box N-CREATE attributes	49
Table 27 - Basic Film Box Status Codes.....	49
Table 28 - Basic Grayscale Image Box N-SET attributes	50
Table 29 - Basic Grayscale Image Box Status Codes	50
Table 30 - Presentation LUT N-CREATE attribute.....	51
Table 31 - Presentation LUT Status Codes.....	52
Table 32 - Used Printer N-EVENT Report attributes.....	52
Table 33 - Mandatory Printer N-GET-RSP, N-EVENT-REPORT-RQ attributes	52
Table 34 - Used Print Job N-EVENT Report attributes	53
Table 35 - Presentation Context Table "Show Device Status"	53
Table 36 - Used Printer N-EVENT Report attributes.....	54
Table 37 - Presentation Context "Update Worklist"	56
Table 38 - Supported Broad Worklist Query Search Key Attributes	56
Table 39 - Basic Worklist C-FIND-RSP Return Key Attributes	57
Table 40 - Status Codes "Update Worklist"	60
Table 41 - Patient based "narrow query" Search Key Attributes.....	61
Table 42 - Presentation Context "Patient Registered"	63
Table 43 - Performed Procedure Step N-CREATE Attributes.....	63
Table 44 - Status Codes "Patient Registered"	65
Table 45 - Performed Procedure Step N-SET Attributes	65
Table 46 - Status Codes "MPPS Update"	68
Table 47 - Default AET Characteristics	69
Table 48 - Remote AE Configuration Items.....	70
Table 49 - General parameter settings and timeouts.....	72
Table 50 - Supported Application Profiles	73
Table 51 - Mapping of Application Profiles Supported	75
Table 52 - STD-GEN-xxx profile supported SOP Classes	76
Table 53 - Supported Single-Byte Character Sets (w/o Code Ext.)	80
Table 54 - Supported Single-Byte Character Sets (with Code Ext.)	81
Table 55 - Supported Multi-Byte Character Sets (w/o Code Ext.).....	81
Table 56 - Supported Multi-Byte Character Sets (with Code Ext.).....	82

Table 57 - Siemens Non-Image IOD - Module Table.....	99
Table 58 - private IOD Attributes that describe the CSA Series Header:	99
Table 59 Private IOD Attributes that describe CSA Non-Images.....	99
Table 60 - Siemens Standard Extended Modules.....	101
Table 61 - private IOD Attributes that describe the CSA Image Header:.....	101
Table 62 - private IOD Attributes that describe MEDCOM Header:.....	101
Table 63 - MEDCOM History Information.....	103
Table 64 - MEDCOM OOG Module.....	103
Table 65 - syngo Report Data	103
Table 66 - Registry of DICOM Data Elements	104
Table 67 - data dictionary of all DICOM IOD attributes where the DICOM standard definitions are extended:.....	105
Table 68 - <i>“Common Status Info evaluation”</i>	111
Table 69 - <i>“Additional Agfa printer Status Info evaluation”</i>	114
Table 70 - <i>“Additional Kodak PACS Link (Imation) printer Status Info evaluation”</i>	114
Table 71 - <i>“Additional Kodak 190 printer Status Info evaluation”</i>	115
Table 72 - <i>“Additional Kodak 2180/1120 printer Status Info evaluation”</i>	115
Table 73 - <i>“Additional Codonics printer Status Info evaluation”</i>	115
Table 74 - <i>“Additional DICOM Execution Status Info evaluation”</i>	116
Table 75 - Additional DICOM Execution Status Information	116

Siemens Healthcare Headquarters

Siemens Healthcare GmbH

Henkestr. 127

91052 Erlangen

Germany

Phone +49 9131 84-0

siemens.com/healthcare

HRT HOOD05162003059650 | © 06.2019, Siemens Healthcare GmbH

On account of certain regional limitations of sales rights and service availability, we cannot guarantee that all products included in this brochure are available through the Siemens sales organization worldwide. Availability and packaging may vary by country and are subject to change without prior notice. Some/All of the features and products described herein may not be available in the United States or other countries. The information in this document contains general technical descriptions of specifications and options as well as standard and optional features that do not always have to be present in individual cases. Siemens reserves the right to modify the design, packaging, specifications and options described herein without prior notice.

Please contact your local Siemens sales representative for the most current information. In the interest of complying with legal requirements concerning the environmental compatibility of our products (protection of natural resources and waste conservation), we recycle certain components. Using the same extensive quality assurance measures as for factory-new components, we guarantee the quality of these recycled components. Note: Any technical data contained in this document may vary within defined tolerances. Original images always lose a certain amount of detail when reproduced. Caution: Federal law restricts this device to sale by or on the order of a physician.